


GTD2000-Tx

Instruction Manual

Revision: 1

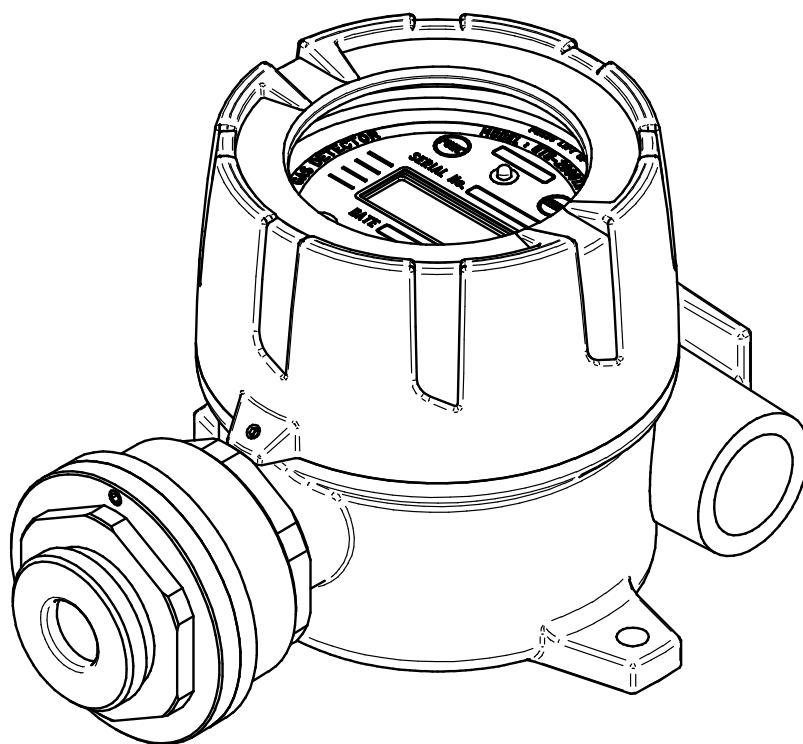

Please read this manual carefully for proper use of the device

Thank you for purchasing the product of us Gastron Co., Ltd.

Gastron has been recognized from many consumers for its top quality and ease of use as a professional company of Gas detectors & Gas Monitors. We are constantly researching and striving to help consumers to find with required products nearby and to develop consumer satisfied Gas detectors. From now on, Gastron detectors will resolve all the troubles you have and satisfy your needs.

This manual contains method for the installation, operation method, and simple maintenance methods on GTD2000-Tx Gas detector. Read it carefully and keep it for further reference in case you have questions.

If there are any problems with our products, please contact us at the address below.

- **Address: 18-8 Dogeumdanji 1gil(Palgogi-dong), Sanglok-gu,
Ansan-city, Gyeonggi-do, Korea,**
- **Tel : 82-31-490-0800**
- **Fax : 82-31-490-0801**
- **URL : www.gastron.com**
- **e-mail : business@gastron.com**

Note

- **Inspection and calibration are recommended at least once every 3 months to ensure accurate operation of the Gas detector using calibration gas depending on the type of gas.**
- **Negligence of periodic inspection and calibration may cause malfunction of the device due to the aging of the Sensor.**
- **Only qualified personnel with professional skills on Gas detector may disassemble the unit if necessary.**
- **For further information on Gas detector inspection and correction, please contact us at our technical department, e-mail or web site.**

This page intentionally left blank

TABLE OF CONTENTS

1. Overview	6
2. Structure	6
3. Specification.....	7
4. Name of Components and Main features	8
4.1. Components.....	8
4.2. Description of components.....	9
5. Terminal wiring diagram	10
5.1. Separation of Detector Body and Cover.....	10
5.2. Main PCB configuration.....	11
5.2.1. Main PCB configuration	11
5.2.2. HART Board configuration.....	12
5.3. Main PCB terminal description and wiring method	14
5.3.1. 4~20mA Source drive type wiring method	15
5.3.2. 4~20mA Sink drive type wiring method.....	16
5.3.3. Connection method with our main Control Unit.....	17
6. Standard Type outside view and Dimensions.....	18
7. Warning light type: Outside view and Dimensions	20
8. Raincover type: Outside view and Dimensions.....	21
9. Menu Configuration Table	22
10. Detector activation Flow and KEY operation.....	25
10.1. Sensor activation Flow	25
10.2. Sensor KEY configuration and description	25
11. Initial status and Menu description	26
11.1. Initial operation status (Power On)	26
11.2. Gas measuring status (Measuring Mode) configuration.....	26
11.3. PROGRAMMABLE MODE Setting.....	27
11.4. CALIBRATION MODE Operation.....	28
11.4.1. Zero Calibration	28
11.4.2. Span Calibration.....	29
11.5. ALARM mode setting	30
11.6. SENSOR DATA MODE configuration.....	32

11.7. Maintenance Mode setting.....	33
11.8. Device Mode setting.....	35
11.9. Version mode configuration	36
11.10. Test mode configuration.....	37
11.11. Inspection mode use.....	38
11.12. Data initialization	38
11.13. Correction data initialization	38
12. Troubleshooting.....	39
13. Caution before installation.....	40
13.1. Selection of installation location (Occupational Safety and Health Law).....	40
13.2. Selection of installation location (High Pressure Gas Safety Management Regulations)	40
13.3. Precaution before installation.....	41
14. Ordering Information	42
15. Revision history	44

1. Overview

GTD2000-Tx toxic gas detector was developed in order to prevent accident by detecting gas leaking in industrial fields such as various toxic gases that are generated in plants manufacturing or using toxic gas, gas storage, or in the manufacturing process.

GTD2000-Tx toxic gas leak detector is installed in areas of risk of leakage; constantly and continuously detects gas leak; displays the measured value in the liquid crystal display (LCD) installed in the detector; and provides DC4-20mA standard output signal.

In addition, the Cable Connection Length of DC4 ~ 20mA standard output signal between sensor element and receiver extends up to 2,500m (When **Cable CVVS or CVVSB 1.5sq** or equivalent is used). This GTD2000-Tx toxic gas detector should be used at an elevation of less than 1000M.

2. Structure

The body of GTD2000-Tx is made of aluminum alloy, and completely explosion-proof (Ex d IIC T6). The product may be installed anywhere risky of combustible gas leak and explosion, displaying the gas leak status in the installation site on the built-in liquid crystal display (LCD) within the sensing unit.

The internal structure is composed of a liquid crystal display unit displaying the measurement; a terminal unit sending the measured value (DC4-20mA) to outside; and a PCB Board. A magnet bar is installed outside, so maintenance work is convenient because calibration is possible from outside using this magnet-bar.

3. Specification


I T E M S	S P E C I F I C A T I O N
Measuring Type	Diffusion
Measuring Value Display	Local Digital LCD or OLED Display
Means Value Display	Back light, 2-line/8-Characters LCD or OLED
Approval	Ex d IIC T6
Detectible Gas	Toxic Gas
Measuring Method	Electro-Chemical Cell
	Heated-semiconductor Cell
Measuring Range	Refer to appendix.
Response Time	90% of full Scale in less than 45 sec
Accuracy	± 3% / Full Scale
Zero Drift	Less than 2% full Scale
Operating Temp.	-20 to 60°C
Operating Humidity	5 to 99% RH (Non-condensing)
Signal Output	Measuring Output: 4 – 20mA.DC / Full Scale
	Test Output: 3mA
	Calibration Output: 3mA
	Fault Output: 2mA
HART® Interface	HART REV7 / Optional Board (Note 1)
Calibration Work	Magnetic interface to configure Alarm
Cable Connection Length	Max. 2,500m : 4-20mA Signal
Power Supply	18 - 31V DC (24V DC / 60mA)
	With alarm device (24V DC / 110mA)
Conduit Connection	1/2" or 3/4"PF, NPT(Standard : 3/4" PF)
Signal Cable Connection	(CVVS or CVVSB 1.5sq ↑ ×3 wires) + Shield
Option	HART® Interface Board
	GTL-100(Explosion-proof Warning Light)
	Rain Cover
Dimensions	136(W) × 166(H) × 110 (D) mm
Weight	App. 1.5kg

[Table 1. GTD2000-Tx Specification]

Note 1) For HART, refer to GTD2000 HART® Field Device Specification

4. Name of Components and Main features

4.1. Components

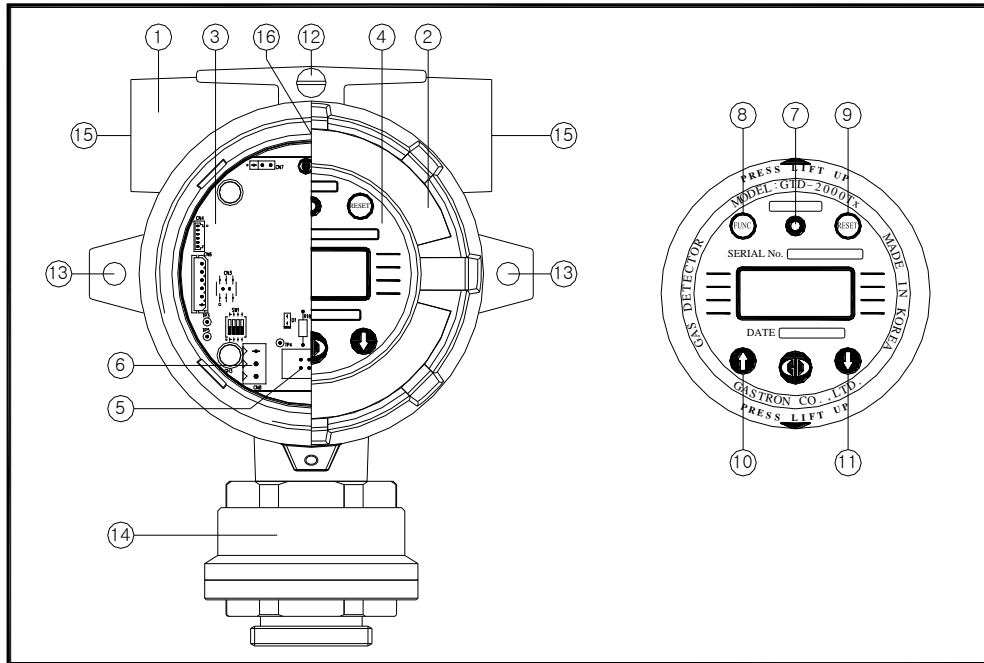

[Figure 1. GTD2000-Tx Components]

No.	Name	No.	Name
1	Detector housing body	9	Reset Switch
2	Detector housing cover	10	↑ (up) Switch
3	AMP(main) PCB	11	↓ (Down) Switch
4	Display parts	12	External Earth Ground(Min 1.5sq Cable)
5	Power/Signal Terminal	13	Mount Holes(ø7)
6	Sensor Terminal	14	Sensor
7	Power LED	15	Conduit Connection
8	Function Switch	16	Internal Ground

[Table 2. Components Reference Table]

4.2. Description of components

No.	Name	Description
1.	Detector Housing Body	Protects Sensor and built-in PCB Board from external environment and shock.
2.	Detector Housing Cover	Is assembled with Detector Housing Body, and has a circular glass top through which LCD displayed Measuring Value can be seen.
3.	AMP PCB	Amplifies the tiny Output generated by Sensor Element, converts it to 4-20mA.DC by converting a standard Output, and transmits the Data to the Display unit.
4.	Display PCB	Displays the Data from AMP / Terminal (Transmitter) PCB to LCD display (Measuring Value), and indicates the power status with the Power Lamp.
5.	Power/Signal Terminal	CN9 is composed of DC18V ~ 31V power supply and a DC 4 ~ 20mA standard Output Connection terminal (VISO, +24V, mA, GND).
6.	Sensor Terminal	CN8 is Sensor Connection Terminal.
7.	Power LED	This Lamp is ON when Power is supplied.
8.	Function Switch	In Measuring Mode, touching this Switch for 2 sec with Magnet-Bar will enter to Function Setting Mode; or will store changed Data in Function Setting Mode.
9.	Reset Switch	Touching this Switch once with Magnet-Bar will cancel the Parameter setting, or return to the previous condition. (Every touch will return the Mode one previous step).
10.	↑ (UP) Switch	Touching this Switch once with Magnet-Bar will convert one step or increase the displayed value in Mode conversion or number change.
11.	↓ (DOWN) Switch	Touching this Switch once with Magnet-Bar will convert one step or decrease the displayed value in Mode conversion or number change.
12.	External Earth Ground	The outside of the Detector should be grounded to protect the circuit from external Noise or strong electric field.
13.	Mount Hole ($\varnothing 7 \times 2ea$)	This Hole is used to secure the Gas Detector on exterior walls and other installation places.
14.	Sensor	Actually detects the gas leak, which is converted to electric signal and transmitted AMP PCB.
15.	Conduit Connection	This is provided for the inlet for power supply and Measuring Output signal. Cable connector has 3/4 ", 1/2" PF or NPT (Default spec. is PF 3/4".)

16.	Internal Ground	The inside of the Detector should be grounded to protect the circuit from external Noise or strong electric field.
-----	------------------------	--

[Table 3. Components details table]


5. Terminal wiring diagram



Warning Never install, uncover, or manipulate the Detector other than authorized personnel or installation/repair service person from Gastron, or serious loss of life and property damage such as fire or explosion may occur. In addition, check around for explosive Gas or flammable substances, followed by turning OFF before any work.


5.1. Separation of Detector Body and Cover

The Gas Detector Cover can be removed by turning the Cover fastening Slotted Set Screw (M4 x 1ea) three to four rotations anti-clockwise using hex wrench (M2), followed by turning the Cover counterclockwise by hand. After the separation of Cover, the LCD indicator appears.

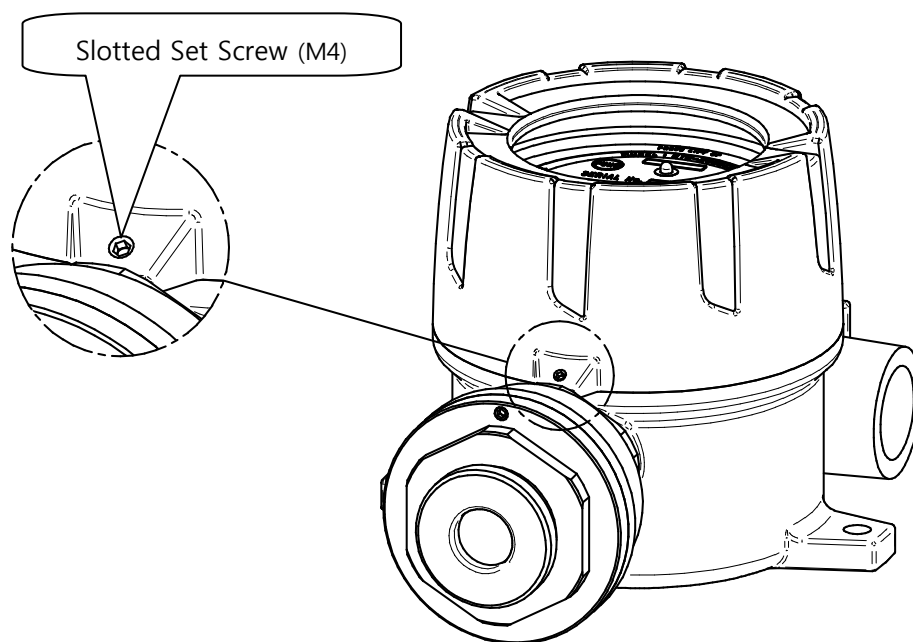

[Figure 2. Slotted Set Screw]

After the Cover removal, remove the Display Part as follows.

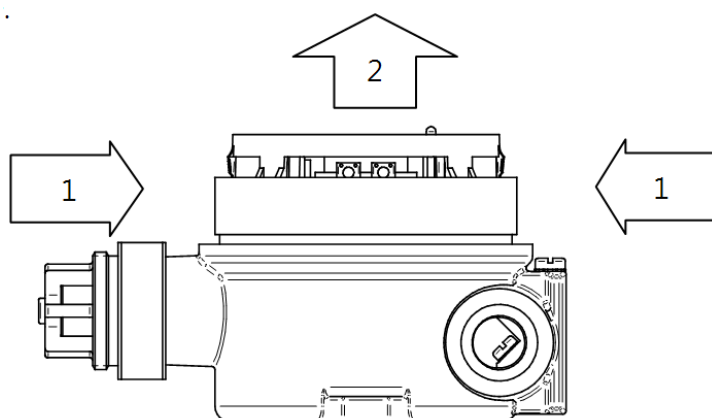


[Figure 3. Display Part removal]

- ① Click the left and right retainer rings on the front of the LCD display inwards at the same time.
- ② While holding, pull the Display Part forward to separate from the Gas detector Body.
- ③ With the Display Part removed, the Main PCB is shown under the Detector Body.

5.2. Main PCB configuration

5.2.1. Main PCB configuration

With the Display Part removed, the Main PCB terminal arrangement is shown as the following Figure.

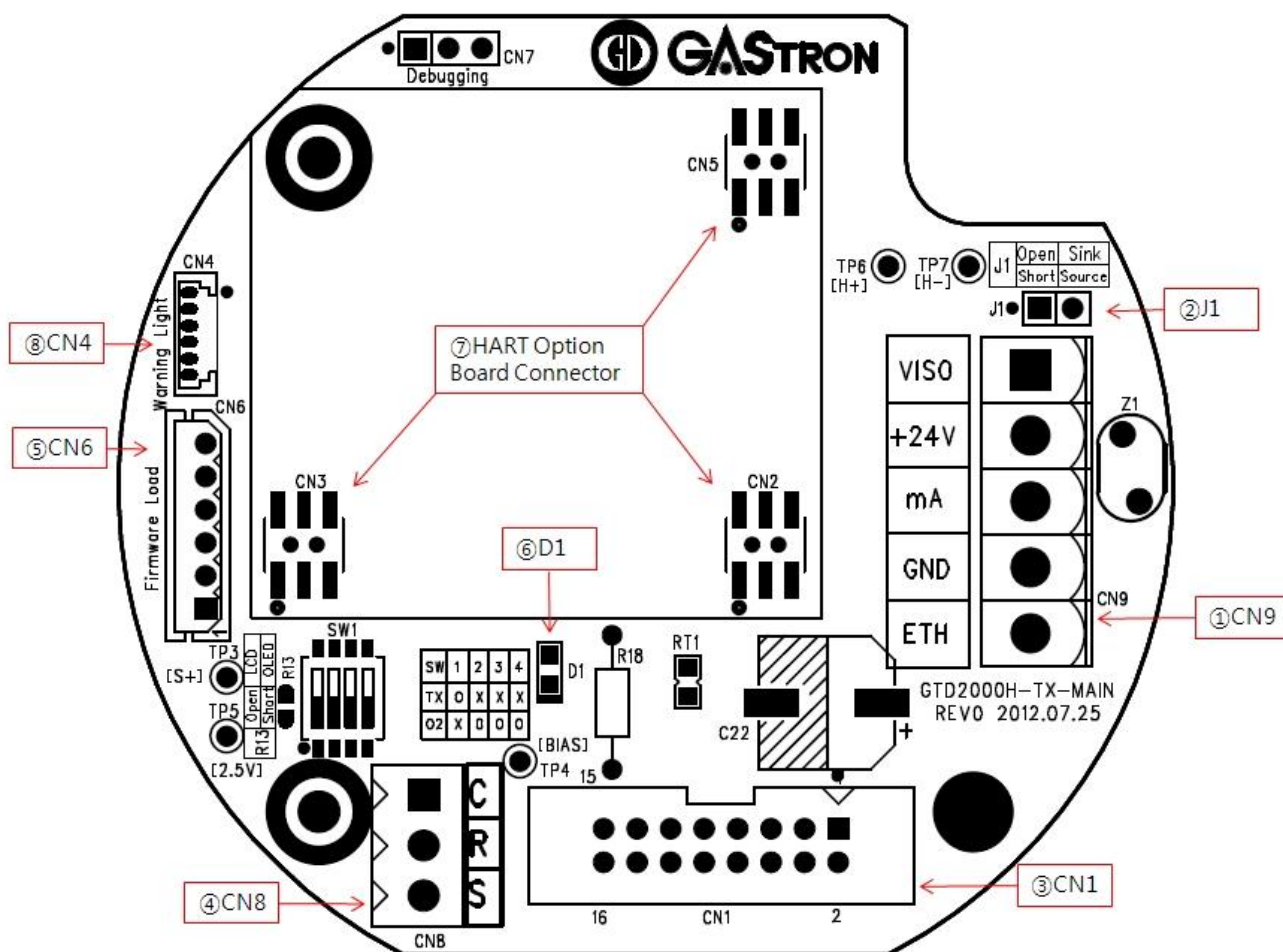


1	HART Board Screw	Constructed using 3Ø Screw
2	Blank Hole	Reserve Hole
3	HART Board	Option Board for HART Interface

[Table 5. HART Board main Parts description]

5.3. Main PCB terminal description and wiring method

If you remove the Display Part, there is the Terminal Block under the Main PCB as shown in the following Figure 6. The Terminal Block can be removed from Main PCB by holding and pulling upward by hand. Unscrew the 5 terminal set screws above the separated **Terminal Block CN9 (VIS, +, mA, -, ETH) Connector** counter-clockwise with a \ominus screwdriver; connect DC18-24V power to +, -; connect Signal Cable to mA; tighten the terminal set screws clockwise to keep the terminals in place; and insert it like before the removal.

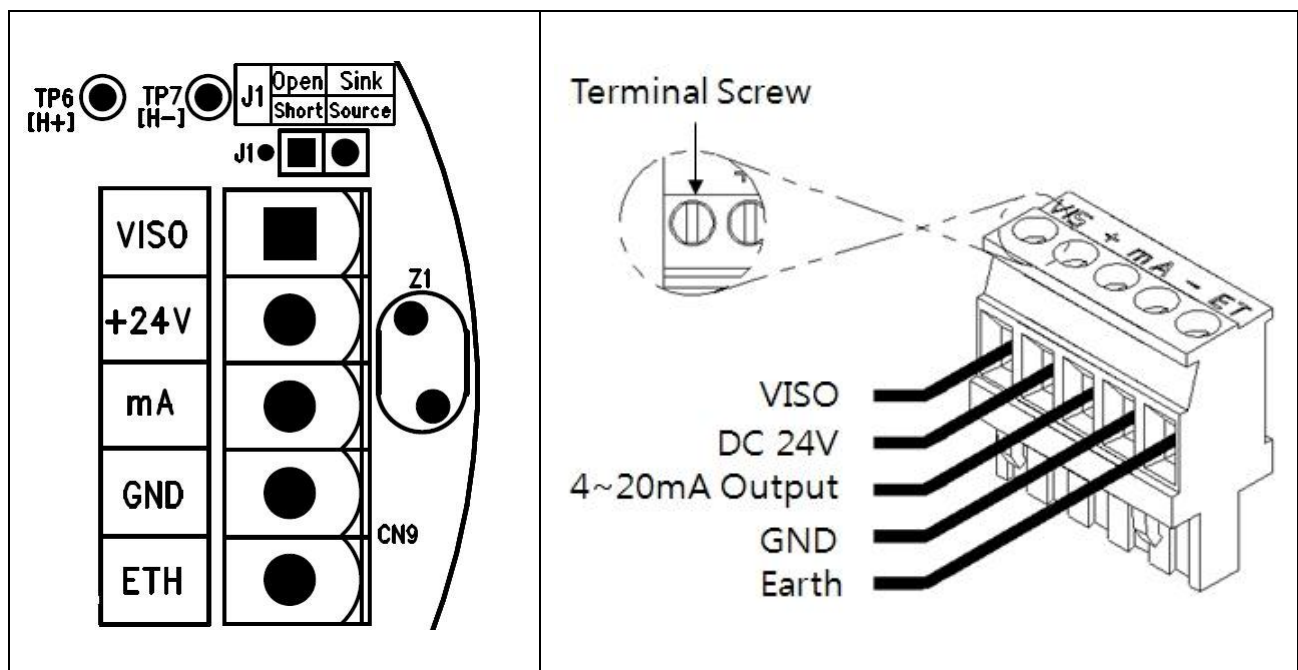

[Figure 6. CN9 Terminal structure]

No	PCB Silk	Pin Name	Description	
			4~20mA Source Drive (J1 Jumper ON)	4~20mA Sink Drive (J1 Jumper OFF)
1	VISO	VIS	N.C	4~20mA Sink In(+)
2	+24V	+	+24V / POWER (+)	
3	mA	mA	4~20mA Source Out	4~20mA Sink Out(-)
4	GND	-	GND / POWER (-)	
5	ETH	ET	EARTH	

[Table 6. CN9 connector description]


Note1) Be sure to use CVVS or CVVSB 1.5sq \uparrow Shield Cable before Terminal construction.

Note2) Fasten Terminals based on +24V of 2Pin to connect the 4Pin Terminal of existing conventional GTD2000-Tx.

5.3.1. 4~20mA Source drive type wiring method

Connect 4-20mA Signal Terminal of PLC to 'mA' of GTD2000-Tx. GND Terminal is used in common with the power. Turn J1 Jumper ON.

※ HART Communicator can be used only in models utilizing HART Option Board.

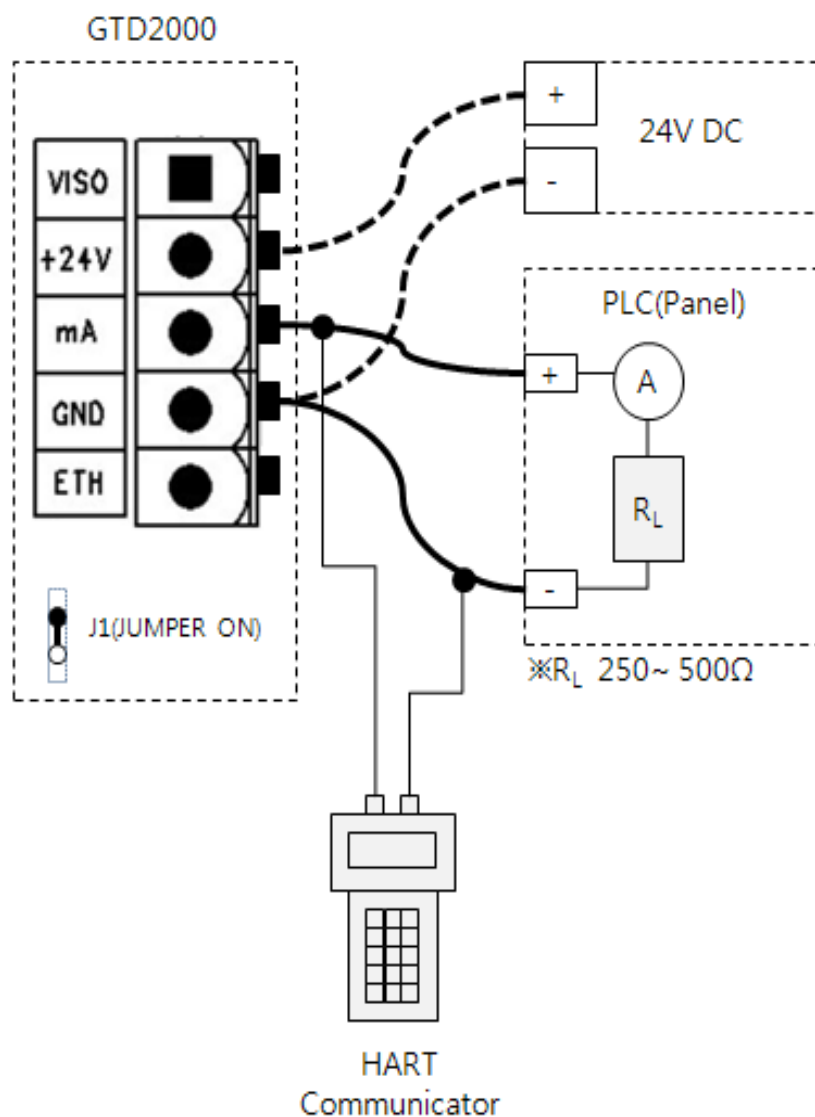


[Figure 7. Analog 4~20mA Source Configuration]

5.3.2. 4~20mA Sink drive type wiring method

Connect 4-20mA Sink Output (+) Terminal of PLC to VISO Terminal; and (-) Terminal to 'mA' Terminal.

Turn J1 Jumper OFF.


※ HART Communicator can be used only in models utilizing HART Option Board.

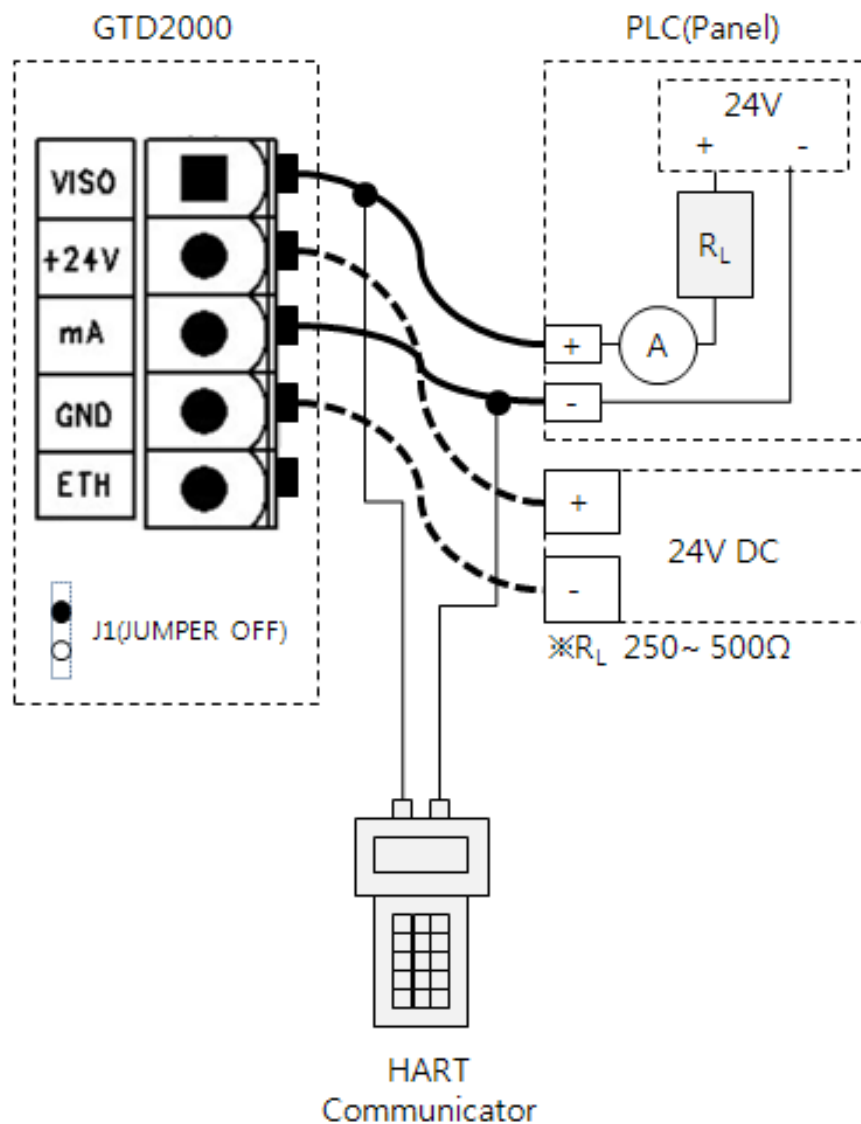


[Figure 8. Analog 4~20mA Sink Configuration]

5.3.3. Connection method with our main Control Unit


Connect CN9 (VISO , + , mA , - , ET) Connection Terminal of the Gas Detector and the Control Unit with reference to the Figure below. (See product manual for each Control Unit.)

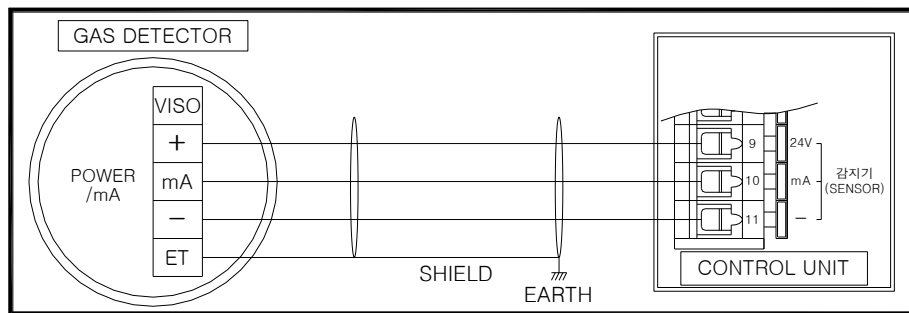

(GTC-100A Series Control unit)

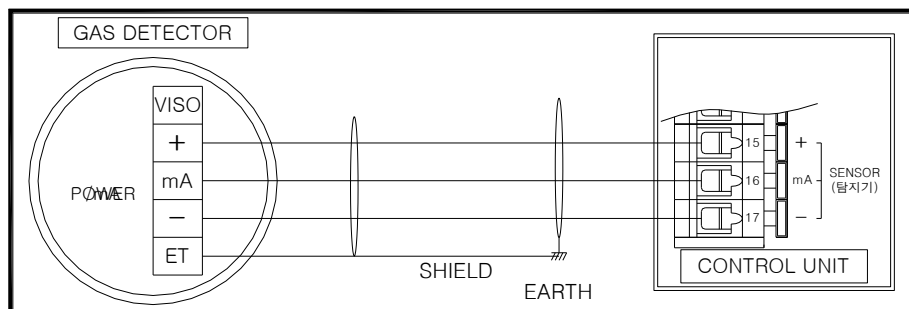


(GTC-200A/210A Series Control unit)

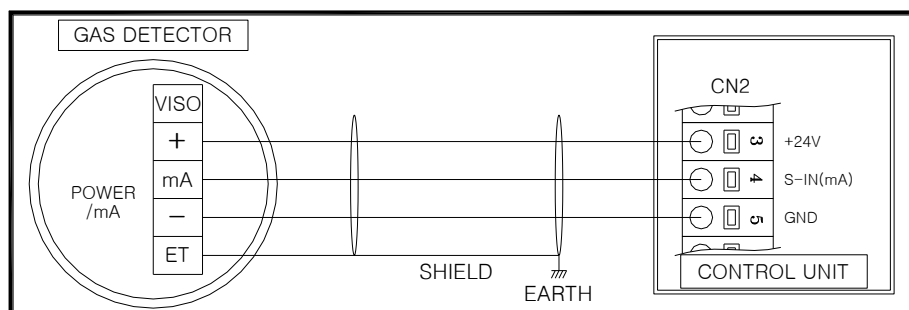


(GTC-510A/520A Series Control unit)

6. Standard Type outside view and Dimensions

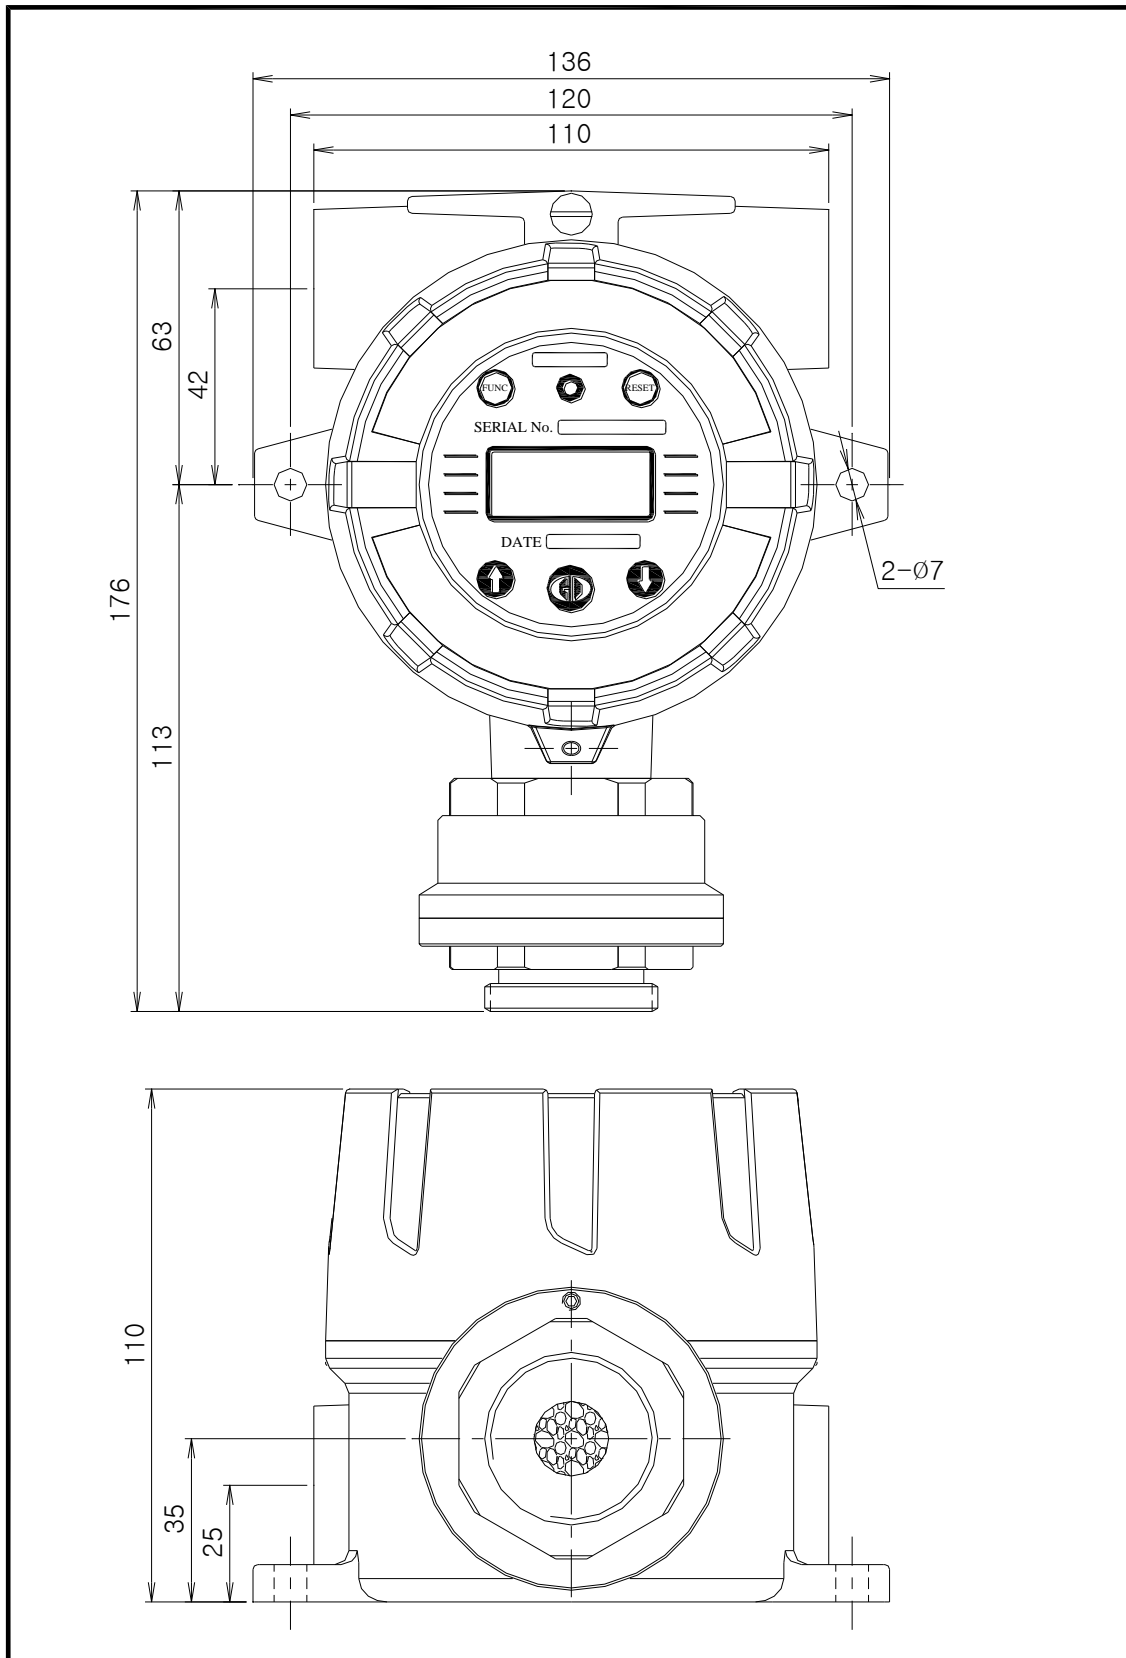


[Figure 9. GTD2000-Tx outside view]

7. Warning light type: Outside view and Dimensions

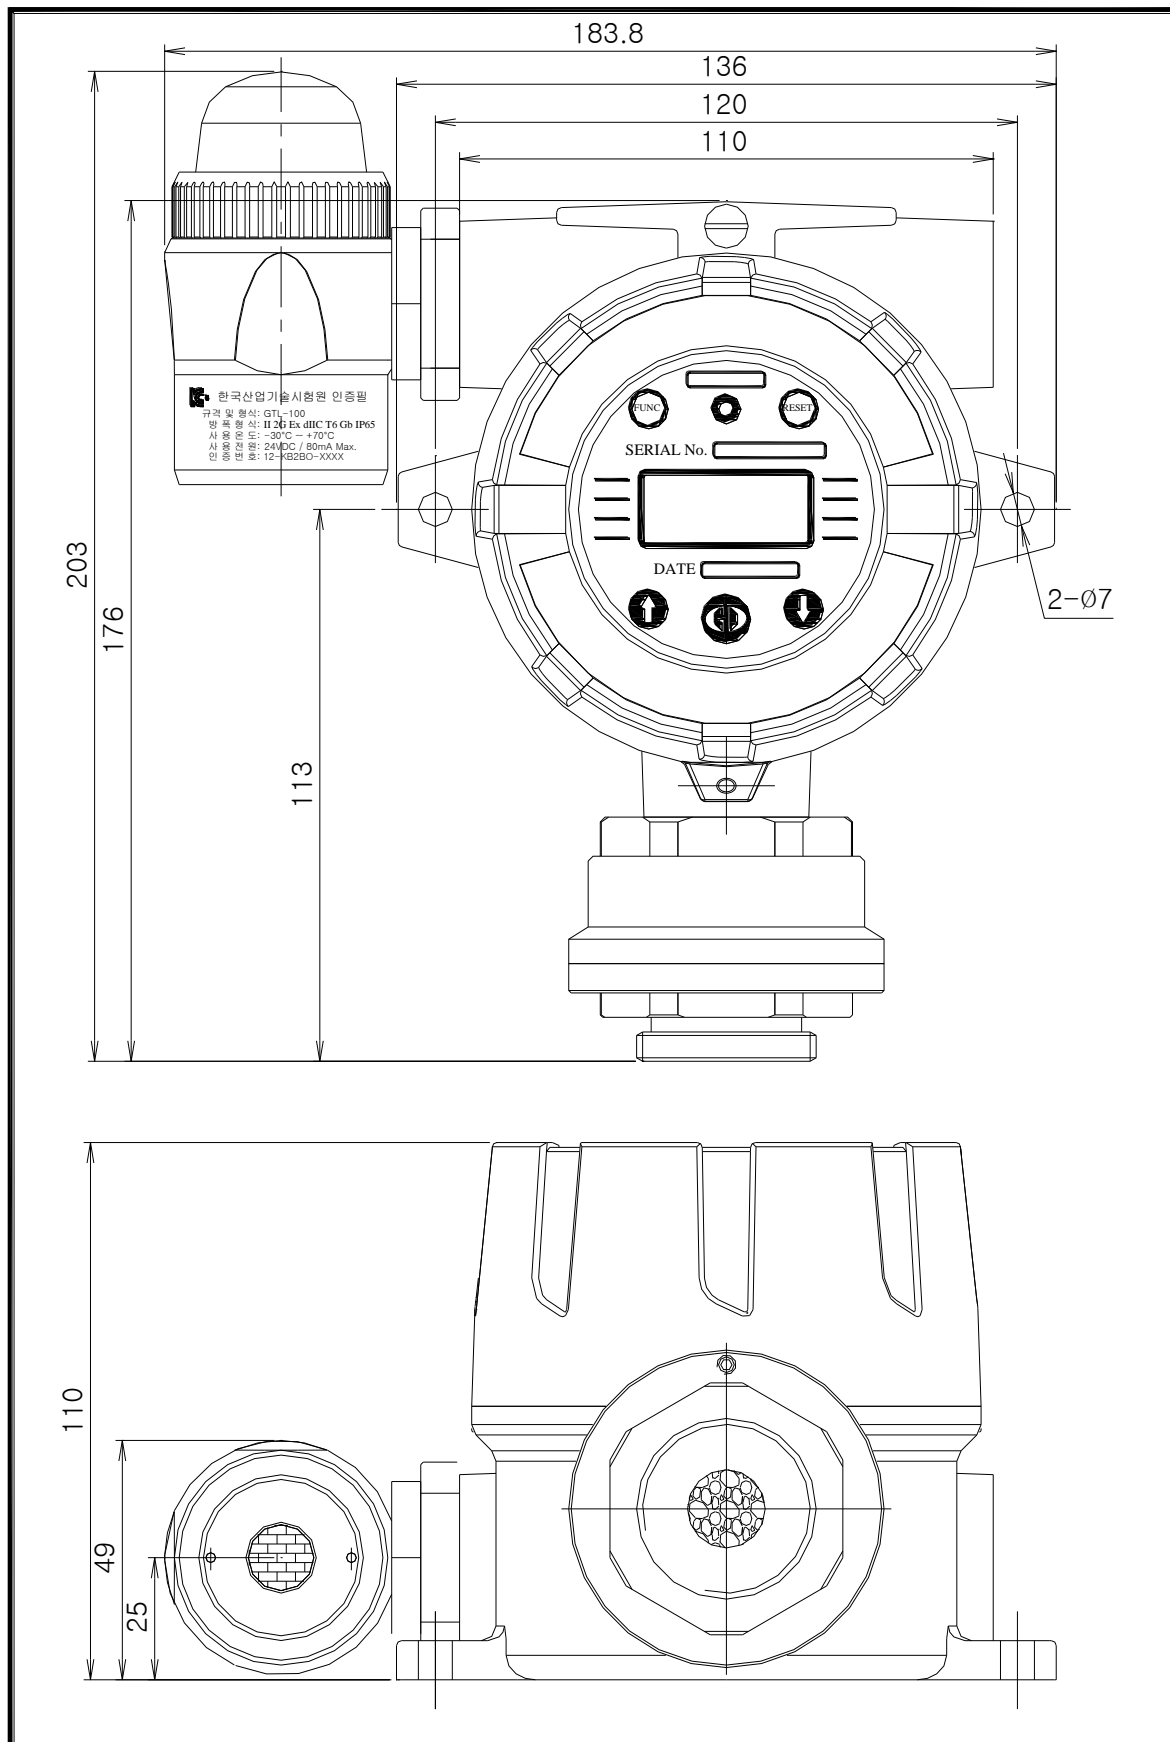

[Figure 10. GTD2000-Tx Warning Light type outside view]

8. Raincover type: Outside view and Dimensions

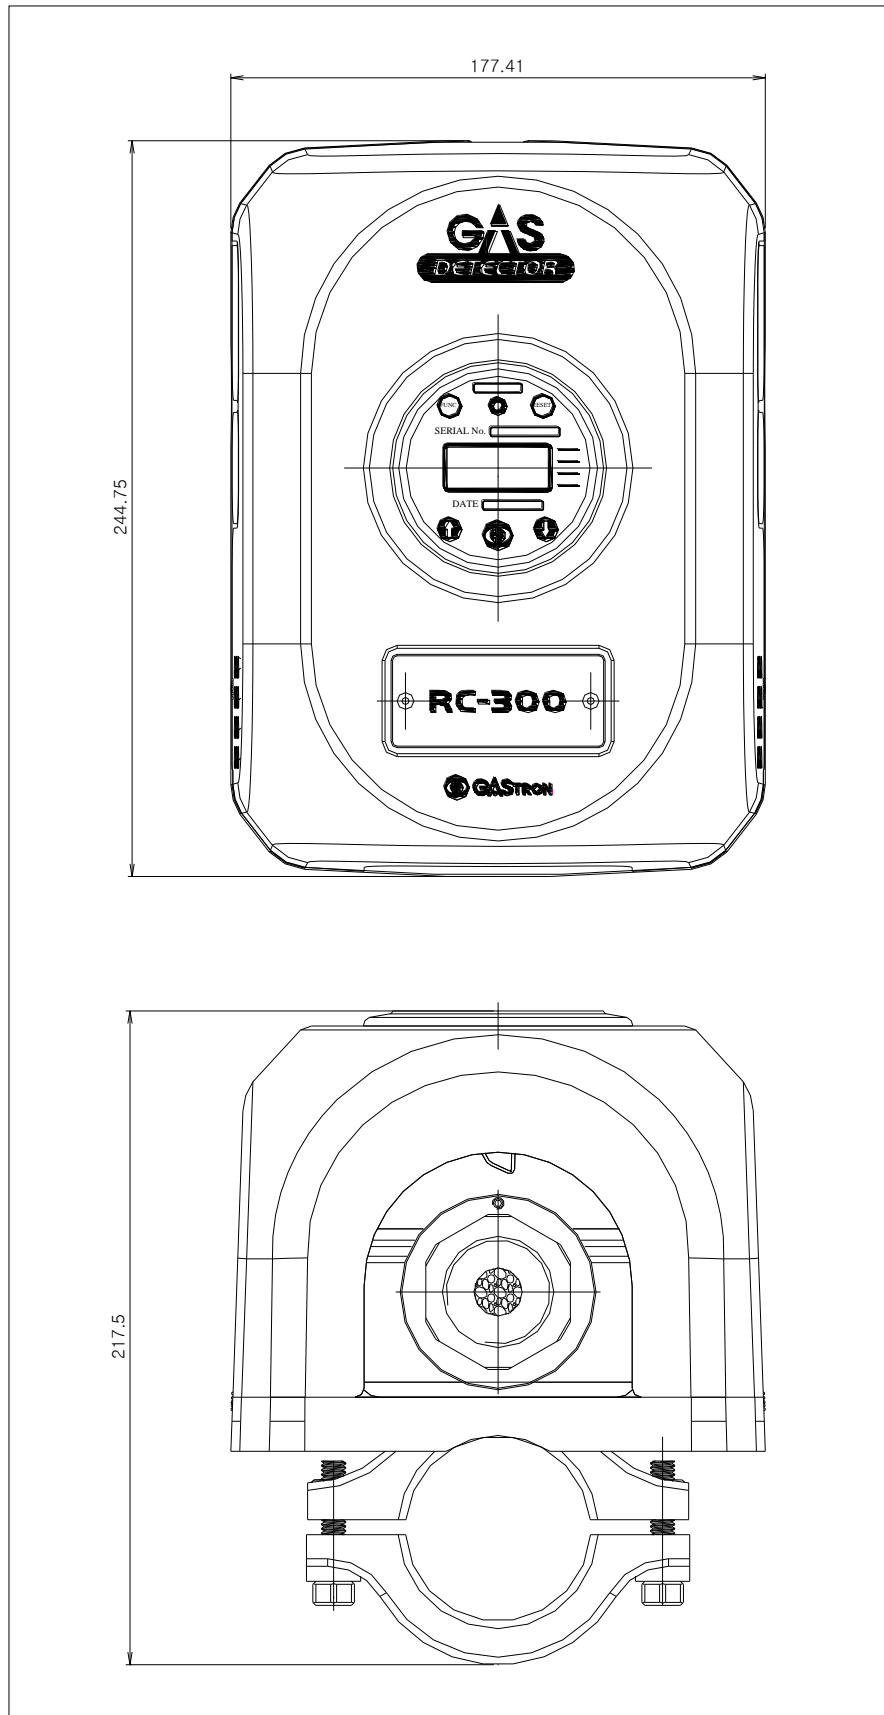

[Figure 11. GTD2000-Tx Raincover type outside view]

9. Menu Configuration Table

Level1	Level2		DEFAULT
	NAME	PARAMETER	
PROGRAM MODE	GAS TYPE (Gas Type)	[DEFIN./USER]	DEFIN.
	GAS SEL (Gas Select)	See Table 8	COMB.
	UNIT SEL (Unit Select)	%/ %LEL/PPM/PPB	%LEL
	D-POINT (Decimal Point)	0.100/1.00/10.0/100	100
	HIGH SCL (High Scale)	1~10000	100
	PASSWORD	00~99	00
CALIBRA. MODE (Calibration Mode)	CALIBRA. [ZERO] (Calibration Zero)	ZERO CAL [NO,YES]	[NO]
		ZERO GAS [0]	
		ZERO >>>> [SUCCESS / FAIL]	
		CAL. DATA [0/ FAIL]	
	CALIBRA. [SPAN] (Calibration Span)	SPAN CAL [NO , YES]	[NO]
		SPAN GAS [0]	
		SPAN SET [50/ FAIL]	50
		SPAN >>>> [SUCCESS / FAIL]	
		CAL. DATA [0]	
ALARM MODE	ALM USED (Alarm Used)	[OFF / ON]	OFF
	AL LATCH (Alarm Latch)	[OFF / ON]	OFF
	A1 LEVEL (Alarm-1 Level)	[1 ~ 9999]	20
	A1 TYPE (Alarm-1 Type)	[INC / DEC]	INC
	A1 DBAND (Alarm-1 Dead Band)	[0.0 ~ 10.0%F]	1.0
	A1 TIME (Alarm-1 Time)	[0~ 60]SEC	1
	A2 LEVEL (Alarm-2 Level)	[1 ~ 9999]	40
	A2 TYPE (Alarm-2 Type)	[INC / DEC]	INC
	A2 DBAND (Alarm-2 Dead Band)	[0.0 ~ 10.0%F]	1.0
	A2 TIME (Alarm-2 Time)	[0~ 60]SEC	1
SENSOR MODE	SEN. OUT (Sensor Output)	[X.X mV]	-
	SEN. S/T (Sensor sensitivity)	[X.X]	-
	MZ / MS (Manual Zero/Span)	X.X / XX.X	1.0 / -100.0
	AZ / AS (Auto Zero / Auto Span)	X.X / XX.X	1.0 / -100.0

Level1	Level2		DEFAULT
	NAME	PARAMETER	
SENSOR MODE	ZR / SR (Zero Rate / Span Rate)	XX.X % / XX.X %	49.9% / 60.0%
	SEN GAIN (Sensor Gain)	[X.X] x G	1.0
	SEN BIAS (Sensor BIAS)	[X.XX V]	-
	TEMP. (Temperature)	[XX 'C]	-
	CURRENT(Sensor Current)	[XXX mA]	-
	24V VIN(GTD2000 Input Power)	[XX.X V]	-
MAINTEN. MODE (Maintenance Mode)	CRO-SENS. (Cross Sensitivity)	[1.00] X G , 0.01~5.0 Adj	1.00
	Z- SKIP (Zero Skip)	[0~10%F]	0.0
	ODT (Operation Delay Time)	[0 ~ 60 SEC]	0
	AUTO – Z (Auto Zero)	[ON / OFF]	ON
	AZ MIN. (AutoZero Minimum)	[1.0~4.0] %F	2.0
	BASE – Z (Base Zero)	[ON / OFF]	ON
	BZ MAX. (BaseZero Maximum)	[0.5~2.0] %F	2.0
	SP. HOLD (Span Hold)	[ON / OFF]	ON
	UNDER EN (Under Enable)	[ON / OFF]	OFF
	SEN CHK. (Sensor Check)	[ON / OFF]	OFF
	SEN-DIR (Sensor Direction)	[INC / DEC]	DEC
	ENG MOD. (Engineer Mode)	[OFF / ON]	OFF
	W/L TYPE (Warning Light Type)	[STEADY / BLINK.]	STEADY
	M.-LEVEL (Maintenance Level)	[0 ~ Full Scale]	0
	EMC T/O (Emergency Time Out)	[ON / OFF]	OFF
DEVICE MODE	HART B/D (Hart Board)	[CHECK / EMPTY]	-
	PADD / mA (Polling Address)	X / (ON/OFF)	-
	DEV-CODE (Device Code)	[0xE1C3]	0xE1C3
	FIX CUR (Fix Current)	[DISABLE / XX.XXmA]	-
	SERIA.NO (Serial Number)	*XXXXXXXX	-
	TAG	GTD-XXXX	GTD-0001
	LONG TAG	GTD-XXXX-LT	GTD-0001-LT
	DESCRIP. (Descriptor)	[GASTRON GTD2000]	[GASTRO >
	MESSAGE	[COMBUSTIBLE]	[COMBUS >
VERSION MODE	F/W REV (Soft Ware)	[REV 6]	-
	E/X H/W (Hard Ware)	[REV 2]	-
	HART DEV (Hart Device)	[REV 1]	-
	HART REV (Hart Revision)	[REV 7]	-
TEST MODE	mA OUT	[ON / OFF]	OFF
	TEST	[0~Full scale]	0

[Table 7. Menu Configuration Table]

※ Gas name Reference Table


No	Gas name	No	Gas name	No	Gas name
00	AN	32	DMDS	64	POCl ₃
01	AsH ₃	33	EDA	65	Si ₂ H ₆
02	B ₂ H ₆	34	EDC	66	SiCl ₄
03	BCl ₃	35	EtsH	67	SiF ₄
04	BF ₃	36	F ₂	68	SiH ₂ .
05	C ₂ H ₂	37	GeH ₄	69	SiH ₄
06	C ₂ H ₄	38	H ₂	70	SO ₂
07	C ₂ H ₄ O	39	H ₂ S	71	SO ₃
08	C ₂ H ₆	40	H ₂ Se	72	TBM
09	C ₃ H ₆	41	HBr	73	TCS
10	C ₃ H ₆ O	42	HC	74	TEOS
11	C ₃ H ₈	43	HCHO	75	THC
12	C ₄ H ₈ O	44	HCl	76	THF
13	C ₅ H ₁₀	45	HCN	77	THT
14	C ₅ H ₁₂	46	HF	78	TMP
15	C ₆ H ₁₄	47	LNG	79	TOLU
16	C ₆ H ₆	48	LPG	80	WF ₆
17	C ₆ H ₆ O	49	MCS	81	OTHER
18	C ₇ H ₈	50	MeCHO		
19	C ₇ H ₈ O	51	MEK		
20	CH ₃ Cl	52	N ₂ H ₄		
21	CH ₃ OH	53	NF ₃		
22	CH ₄	54	NG		
23	CiF ₃	55	NH ₃		
24	Cl ₂	56	NMP		
25	CLF ₃	57	NO		
26	CO	58	NO ₂		
27	CO ₂	59	O ₂		
28	COCl ₂	60	O ₃		
29	COMB.	61	PCL ₃		
30	DCS	62	PH ₃		
31	DMC	63	PhoH		

[Table 8. Gas name table]

10. Detector activation Flow and KEY operation

10.1. Sensor activation Flow

- Timeout of Level1 and Level2 is 10 seconds, and 1 hour in the Calibration and Test Mode of Level2.

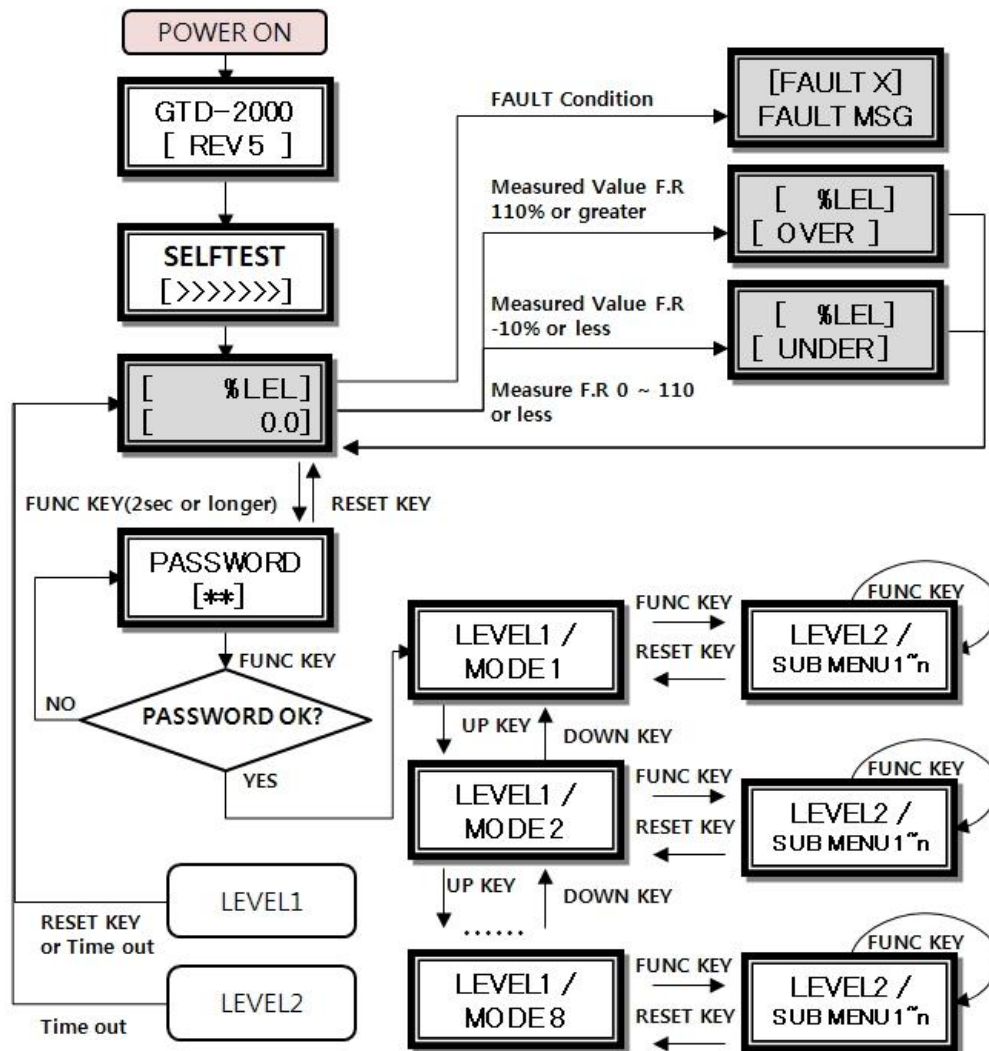

[Figure 12. Sensor workflow]

10.2. Sensor KEY configuration and description



Item	Name	Description
FUNC	Function Key	Sensor Mode entry function (more than 2 seconds of touch with Magnet-bar in Measuring Mode). Entry to the next step of Level2 and storage of setting value.
RESET	Reset Key	Moving back to the previous step before the entered LEVEL
↑	Up Key	Change to the next step after LEVEL1, and plus change of Level2 setting.
↓	Down Key	Change to previous step before LEVEL1; minus change of Level2 setting.

※ Sensor Power ON followed by simultaneous input of Reset Key and Function Key will result in Factory Set in internal setting.






11. Initial status and Menu description

11.1. Initial operation status (Power On)

After wiring of and power supplying to Power Terminal on MAIN PCB board, the following information will be displayed on the LCD display. About 30 minutes of stabilization time is required about 30 minutes' stabilization time is required; normal operation begins after full stabilization.

	<ul style="list-style-type: none"> ➤ After the Power ON, the model name and product firmware Revision number is displayed on LCD (OLED).
	<ul style="list-style-type: none"> ➤ Self test runs for one minute, and the '>' character in second row indicates the progress.

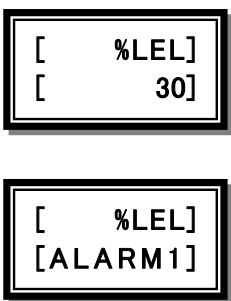11.2. Gas measuring status (Measuring Mode) configuration

	<ul style="list-style-type: none"> ➤ Operation is as follows in Normal state. ➤ In the first row, Measuring GAS NAME and Measuring GAS Unit are displayed alternately every second; in the second row, current Measuring Value is displayed. ➤ Touching 'Func' Key with Magnet-bar for 2 seconds in current screen will change to Setting Mode. ※ During HART communications, '** character is displayed on the left side of the 1st row. ※ When ENG. Mode is ON, '<' character is marked on the left side of the 2nd row.
	<ul style="list-style-type: none"> ➤ The operation is as follows when 1st or 2nd Alarm has occurred (ALARM EN item of Maintenance Mode must be ON to enable the operation). ➤ The 1st row is operated the same as in Normal mode; in the 2nd row, ALARM messages and Gas Measuring Value are displayed alternately every 1 second. ➤ When GTL100 Explosion-proof Warning Light is installed, the red LED and Buzzer are blinking every second in the 1st Alarm; no flashing occurs in the 2nd Alarm. ➤ Alarm condition continues unless it was released using Reset key if the Latch is on during Alarm function.
	<ul style="list-style-type: none"> ➤ If the entered Gas Measuring Value is more than 10% higher than set High Scale, the word "OVER" is displayed blinking every 1 second. ➤ At this time 4~20mA is operated as 21.6mA.
	<ul style="list-style-type: none"> ➤ If the entered Gas Measuring Value is less than 10% lower, the word "UNDER" is displayed blinking every 1 second; 4 ~ 20mA is operated below 2mA. ※ This feature is operated only when UNDER button is ON.
	<ul style="list-style-type: none"> ➤ If there is any problem with the device, the Fault number and message will be displayed. ➤ At this time, the 4 ~ 20mA is operated below 2mA. ➤ The left Mode is displayed when Fault1 sensor is not equipped.

11.3. PROGRAMMABLE MODE Setting

Touching the "RESET" switch in Program Mode screen will revert to Measuring Condition; and touching "RESET" switch in each Program Setting screen will revert to "PROGRAM MODE".

<div style="border: 2px solid black; padding: 5px; text-align: center;"> PASSWORD [**] </div>	<ul style="list-style-type: none"> ➤ Touching "FUNC" switch with Magnet-bar for 2 seconds in Measuring Condition will enter the Password mode. ➤ Touch the "FUNC" switch after setting password using "↑" or "↓" switch.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> PROGRAM MODE </div>	<ul style="list-style-type: none"> ➤ It will enter Program Mode if the password is right. ➤ The Mode will change in the specified order on every touching of "↑" or "↓" switch. (PROGRAM -> CALIABRA. -> ALARM -> SENSOR -> MAINTEN. -> DEVICE -> VERSION -> TEST)
<div style="border: 2px solid black; padding: 5px; text-align: center;"> GAS TYPE [DEFIN.] </div>	<ul style="list-style-type: none"> ➤ It is Gas Type Setting Mode: Gas Type is changed every time "↑" or "↓" switch is touched (DEFIN. / USER). ➤ DEFIN. Shorts for Define, and is selected to use set Gas Type. USER is selected for the user to set the gas Type directly. ➤ Touching "FUNC" switch when desired Gas Type is displayed will define the Gas Type and enter the next Program Mode.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> GAS SEL [COMB.] </div>	<ul style="list-style-type: none"> ➤ It is Gas name Setting Mode: Gas name is changed every time "↑" or "↓" switch is touched (DEFIN. / USER).
<div style="border: 2px solid black; padding: 5px; text-align: center;"> USER GAS [■SER] </div>	<ul style="list-style-type: none"> ➤ When Gas Type is set to DEFIN., Gases listed in Table 8 may be selected for use; when Gas Type is set to USER, the gas name is defined using 5 character keys. Numbers, uppercase alphabetic letters, space, and dot can be used. If the location moves to input letter, black box cursor is displayed like the Figure.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> UNIT SEL [%LEL] </div>	<ul style="list-style-type: none"> ➤ Gas Measuring Unit Mode. Gas measuring unit is changed with touching of "↑" or "↓" switch each time (% /% LEL / PPM / PPB). ➤ Touching "FUNC" switch will set the displayed Gas Measuring Unit desired, and will enter the next Program item.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> D-POINT [100] </div>	<ul style="list-style-type: none"> ➤ Decimal point setting Mode. The decimal point is changed on touching of "↑" or "↓" switch each time (0.100/1.00/10.0/100). ➤ The desired and displayed decimal point is defined with the touch of "FUNC" switch; and the next Program item will be entered.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> HIGH SCL [100] </div>	<ul style="list-style-type: none"> ➤ High Scale setting Mode to be displayed in Full Range. The Scale value is increased or decreased on touching of "↑" or "↓" switch (1 ~ 10000). ➤ Touching "FUNC" switch will define the displayed and desired High scale and enter the next Program.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> PASSWORD [00] </div>	<ul style="list-style-type: none"> ➤ Password setting Mode. Password is checked when entering Parameter Program Mode or Maintenance Mode. ➤ "↑" switch or "↓" switch is used to set the password; touching "FUNC" switch will define the password and enter the next Program Item

11.4. CALIBRATION MODE Operation

Due to the nature of the Gas detector, stabilization time of at least 30 minutes is required after power supply; management criteria may vary depending on the field condition.

11.4.1. Zero Calibration

<div style="border: 2px solid black; padding: 5px; text-align: center;"> PASSWORD [**] </div>	<ul style="list-style-type: none"> ➤ Touching "FUNC" switch with Magnet-bar for 2 seconds in Measuring Condition will enter the Password mode. ➤ Touch the "FUNC" switch after setting password using "↑" or "↓" switch.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> CALIBRA. MODE </div>	<ul style="list-style-type: none"> ➤ Select "CALIBRA. MODE" by touching "↑" or "↓" switch. ➤ Touching "FUNC" switch when "CALIBRA. MODE" is displayed will enter Calibration Mode. ➤ Measuring Condition will return on touching "RESET" switch.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> CALIBRA. [ZERO] </div>	<ul style="list-style-type: none"> ➤ Touching "FUNC" switch when "CALIBRA. MODE" is displayed will select Calibration Mode. ➤ Select [ZERO] by touching "↑" or "↓" switch. Now, touch "FUNC" switch to enter Zero Calibration mode.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> ZERO CAL [NO] </div>	<ul style="list-style-type: none"> ➤ Select [YES] by touching "↑" or "↓" switch. Now, touch "FUNC" switch to carry out Zero Calibration.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> ZERO GAS [0] </div>	<ul style="list-style-type: none"> ➤ Inject clean air or 100% nitrogen gas into the sensor using a calibration device at 1000mL/min for a minute; touch "FUNC" Switch when Measuring Value was stabilized to carry out Zero calibration automatically.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> ZERO >> [SUCESS] </div>	<ul style="list-style-type: none"> ➤ After a successful Zero calibration, "ZERO SUCCESS" will be displayed on LCD Display for 2 seconds, and the mode will switch to "CALIBRATION DATA" Mode.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> ZERO >> [FAIL] </div>	<ul style="list-style-type: none"> ➤ When Zero Calibration does not succeed, "ZERO FAIL" is displayed for two seconds, and it will switch to "CALIBRATION DATA" Mode. ➤ ZERO FAIL happens when sensor input exceeds 70% of ADC input range.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> CAL.DATA [0] </div>	<ul style="list-style-type: none"> ➤ It's the Mode displaying Measuring Value after Calibration and the function to check if the calibration was performed normally. ➤ If Failed, FAIL Text and current Measuring Value will be displayed at 1-second intervals. ➤ "CALIBRATION MODE" returns on touching "RESET" Switch.

11.4.2. Span Calibration

※ Entering Calibration Mode is same as Zero Calibration.

<div style="border: 2px solid black; padding: 5px; text-align: center;"> CALIBRA. MODE </div>	<ul style="list-style-type: none"> ➤ Select "CALIBRA. MODE" by touching "↑" or "↓" switch. ➤ Touching "FUNC" switch when "CALIBRA. MODE" is displayed will enter Calibration Mode. ➤ Measuring Condition will return on touching "RESET" switch.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> CALIBRA. [SPAN] </div>	<ul style="list-style-type: none"> ➤ Select [SPAN] by touching "↑" or "↓" switch. Now, touch "FUNC" switch to enter Span Calibration mode.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> SPAN CAL [NO] </div>	<ul style="list-style-type: none"> ➤ Select [YES] by touching "↑" or "↓" switch. Now, touch "FUNC" switch to carry out Span Calibration.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> SPAN GAS [50] </div> <div style="border: 2px solid black; padding: 5px; text-align: center;"> [50] [50] </div>	<ul style="list-style-type: none"> ➤ Inject standard gas into the Sensor using a calibration device at 500mL/min for 90 sec; touch "FUNC" Switch when Measuring Value was stabilized to enter the next Mode. ➤ When HOLD function of Maintenance Mode is ON, the maximum value of the current SPAN gas is HOLD, and the HOLD value is displayed in the 1st row. ➤ In the 2nd row is the current Measuring Value displayed.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> SPAN SET [50] </div> <div style="border: 2px solid black; padding: 5px; text-align: center;"> SPAN SET LOW FAIL </div> <div style="border: 2px solid black; padding: 5px; text-align: center;"> SPAN SET HIGH FAIL </div>	<ul style="list-style-type: none"> ➤ It's the Mode to set the standard gas value, which is set by touching "↑" Switch or "↓" Switch if there's no Fail message. ➤ Fail message is displayed as follows when injected standard gas value is not normal. Fail message and Span set value are displayed alternately. <ul style="list-style-type: none"> ① "LOW FAIL" occurs when the difference of injected Gas value and ZERO Calibration value is less than 1%. ② "HIGH FAIL" occurs when injected Gas value is greater than 95% of the entire ADC input range. ③ "RNG FAIL" occurs when injected Gas value is operating as currently set SPAN value and exceeds more than 95% of the ADC's input range. The FAIL message is lifted when the normal operation resumes through SPAN value adjustment.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> SPAN >> [SUCESS] </div> <div style="border: 2px solid black; padding: 5px; text-align: center;"> SPAN >> [FAIL] </div>	<ul style="list-style-type: none"> ➤ SPAN calibration is performed after setting standard gas value and touching "FUNC" Switch. If the automatic SPAN calibration is successful, "SPAN SUCCESS" is displayed on LCD Display for 2 sec, and the mode is converted to "CAL DATA" Mode. ➤ When Zero Calibration does not succeed, "SPAN FAIL" is displayed for two seconds, and it will switch to "CAL DATA" Mode.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> CALDATA [0] </div>	<ul style="list-style-type: none"> ➤ It's the Mode displaying Measuring Value after Calibration and the function to check if the calibration was performed normally. ➤ "CALIBRATION MODE" returns on touching "RESET" Switch.

11.5. ALARM mode setting

<div style="border: 1px solid black; padding: 5px; text-align: center;"> PASSWORD [**] </div>	<ul style="list-style-type: none"> ➤ Touching "FUNC" switch with Magnet-bar for 2 seconds in Measuring Condition will enter the Password mode. ➤ Touch the "FUNC" switch after setting password using "↑" or "↓" switch.
<div style="border: 1px solid black; padding: 5px; text-align: center;"> ALARM MODE </div>	<ul style="list-style-type: none"> ➤ Select "ALARM MODE" by touching "↑" or "↓" switch. ➤ Touching "FUNC" switch when "ALARM MODE" is displayed will enter Alarm setting Mode. ➤ Measuring Condition will return on touching "RESET" switch.
<div style="border: 1px solid black; padding: 5px; text-align: center;"> ALM USED [OFF] </div>	<ul style="list-style-type: none"> ➤ An item that turns ON / OFF Alarm Mode setting. ➤ Changes ON / OFF status by touching "↑" Switch or "↓" Switch. When it's ON, Alarm function and Alarm Mode can be set. ➤ When it's ON only, the GTL100 Explosion-proof Warning Light can be used. ➤ "FUNC" Switch shall be touched to enter into the next mode.
<div style="border: 1px solid black; padding: 5px; text-align: center;"> AL LATCH [OFF] </div>	<ul style="list-style-type: none"> ➤ It's a Mode setting Reset method after Alarm1 action; touching the "↑" Switch or "↓" Switch toggles "ON" and "OFF". ➤ "OFF" setting automatically resets Alarm; "ON" setting resets Alarm only when Reset Switch is ON. ➤ When the desired MODE is played, it is set by touching "FUNC" Switch; and the next Alarm setting item is entered.
<div style="border: 1px solid black; padding: 5px; text-align: center;"> A1 LEVEL [20] </div>	<ul style="list-style-type: none"> ➤ Alarm1 level setting Mode. The Alarm1 level is increased or decreased on touching of "↑" or "↓" switch (1 ~ 10000). ➤ Touching "FUNC" switch will define the Alarm1 level when desired Alarm1 level is displayed.
<div style="border: 1px solid black; padding: 5px; text-align: center;"> A1 TYPE [INC] </div> <div style="border: 1px solid black; padding: 5px; text-align: center;"> A1 TYPE [DEC] </div>	<ul style="list-style-type: none"> ➤ This MODE sets the direction of Alarm1 Mode; touching the "↑" Switch or "↓" Switch toggles the display of "INC" or "DEC". ➤ "INC" Mode is operating when Alarm value is greater than or equal to Alarm setting value; "DEC" Mode is operating when Alarm value is less than or equal to Alarm setting value; ➤ The desired Mode is set by touching "FUNC" Switch when the desired Mode is displayed; and the next item is entered.
<div style="border: 1px solid black; padding: 5px; text-align: center;"> A1 DBAND [1.0]%F </div>	<ul style="list-style-type: none"> ➤ The Mode sets Dead band where Alarm1 operates; the value is set using "↑" or "↓" key. ➤ Alarm1 is operated at Alarm1 level plus Dead band value or greater; Alarm1 is released at Alarm1 level minus Dead band value or less. ➤ Touching the "FUNC" Switch will set Alarm1 value when desired Dead band is displayed. The next item will be entered.

<div style="border: 2px solid black; padding: 5px; text-align: center;"> A1 TIME 1 SEC </div>	<ul style="list-style-type: none"> ➤ It's the function to prevent the transient malfunction of Alarm1 due to external shock and noise. Time can be set within the range of 0 ~ 60sec. ➤ Alarm1 delay is increased or decreased by 1 sec at every push of "↑" or "↓" key. ➤ When the desired Alarm1 delay time is displayed, press the "FUNC" key to set the Alarm1 delay time and to enter next item. ➤ Example) At alarm set value=20%, and LEL / Delay time=5 Sec, an alarm occurs when the Measuring Value exists 5 sec more than the alarm setting value based on 20% LEL. No alarm will occur less than 5 sec.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> A2 LEVEL [40] </div>	<ul style="list-style-type: none"> ➤ Alarm2 level setting Mode. The Alarm2 level is increased or decreased on touching of "↑" or "↓" switch. ➤ Touching "FUNC" switch will define the Alarm2 level when desired Alarm2 level is displayed.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> A2 TYPE [INC] </div> <div style="border: 2px solid black; padding: 5px; text-align: center;"> A2 TYPE [DEC] </div>	<ul style="list-style-type: none"> ➤ This MODE sets the direction of Alarm2 Mode; touching the "↑" Switch or "↓" Switch toggles the display of "INC" or "DEC". ➤ "INC" Mode is operating when Alarm value is greater than or equal to Alarm setting value; "DEC" Mode is operating when Alarm value is less than or equal to Alarm setting value; ➤ The desired Mode is set by touching "FUNC" Switch when the desired Mode is displayed; and the next item is entered.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> A2 DBAND [1.0]%F </div>	<ul style="list-style-type: none"> ➤ The Mode sets Dead band where Alarm2 operates; the value is set using "↑" or "↓" key. ➤ Alarm2 is operated at Alarm2 level plus Dead band value or greater; Alarm2 is released at Alarm2 level minus Dead band value or less. ➤ Touching the "FUNC" Switch will set Alarm2 value when desired Dead band is displayed. The next item will be entered.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> A2 TIME 1 SEC </div>	<ul style="list-style-type: none"> ➤ It's the function to prevent the transient malfunction of Alarm2 due to external shock and noise. Time can be set within the range of 0 ~ 60sec. ➤ Alarm2 delay is increased or decreased by 1 sec at every push of "↑" or "↓" key. ➤ When the desired Alarm2 delay time is displayed, press the "FUNC" key to set the Alarm2 delay time and to enter next item. ➤ Example) At alarm set value : 20%, and LEL / Delay time : 5 Sec, an alarm occurs when the Measuring Value exists 5 sec more than the alarm setting value based on 20% LEL. No alarm will occur less than 5 sec.

11.6. SENSOR DATA MODE configuration

It's the Mode displaying current Sensor value and Calibration condition. Setting is not possible.

<div>PASSWORD [**]</div>	<ul style="list-style-type: none"> ➤ Touching "FUNC" switch with Magnet-bar for 2 seconds in Measuring Condition will enter the Password mode. ➤ Touch the "FUNC" switch after setting password using "↑" or "↓" switch.
<div>SENSOR MODE</div>	<ul style="list-style-type: none"> ➤ Select "SENSOR MODE" by touching "↑" or "↓" switch. ➤ Touching "FUNC" switch when "SENSOR MODE" is displayed will enter Alarm setting Mode. ➤ Measuring Condition will return on touching "RESET" switch.
<div>SEN. OUT 10.0mV</div>	<ul style="list-style-type: none"> ➤ Displays sensor voltage value being currently measured. ➤ Touching "FUNC" Switch will enter the next item.
<div>SEN. S/T 0.1mV</div>	<ul style="list-style-type: none"> ➤ It displays the difference of current Sensor Measuring Value and ZERO Calibrated Measuring Value. ➤ The unit of the displayed value is mV. ➤ Touching "FUNC" Switch will enter the next item.
<div>MZ 1.0 MS -100.0</div>	<ul style="list-style-type: none"> ➤ It displays the normal Calibration ZERO and SPAN Measuring Value. ➤ The unit of the displayed value is mV. ➤ Touching "FUNC" Switch will enter the next item.
<div>AZ 1.0 AS -100.0</div>	<ul style="list-style-type: none"> ➤ It displays the automatic Calibration ZERO and SPAN Measuring Value. ➤ The corresponding values are automatically updated in Regular Calibration. ➤ The unit of the displayed value is mV. ➤ Touching "FUNC" Switch will enter the next item.
<div>ZR 49.9% SR 60.0%</div>	<ul style="list-style-type: none"> ➤ This Mode displays the percentage variation of current Calibration voltage and Sensor ADC maximum voltage. ➤ Touching "FUNC" Switch will enter the next item.
<div>SEN GAIN [1.0] x G</div>	<ul style="list-style-type: none"> ➤ Output Mode of Sensor Output values multiplied by the corresponding setting value. ➤ The range of Setting is from 0.1 to 5.0.
<div>SEN BIAS [3.18V]</div>	<ul style="list-style-type: none"> ➤ This Mode displays the sensor bias applied to the sensor. ➤ Touching "FUNC" Switch will enter the next item.
<div>TEMPER [25' C]</div>	<ul style="list-style-type: none"> ➤ This Mode displays the temperature measured in the Sensor. ➤ Touching "FUNC" Switch will enter the next item.
<div>CURRENT [176mA]</div>	<ul style="list-style-type: none"> ➤ This Mode measures the current consumption in the Sensor. ➤ Touching "FUNC" Switch will enter the next item.
<div>24V VIN [24.0V]</div>	<ul style="list-style-type: none"> ➤ It measures the Sensor input 24V power supply. ➤ SENSOR MODE will return on touching of "FUNC" Switch.

11.7. Maintenance Mode setting

※  **Only authorized personnel are allowed to perform these settings.**

<div style="border: 1px solid black; padding: 5px; text-align: center;"> PASSWORD [**] </div>	<ul style="list-style-type: none"> ➤ Touching "FUNC" switch with Magnet-bar for 2 seconds in Measuring Condition will enter the Password mode. ➤ Touch the "FUNC" switch after setting password using "↑" or "↓" switch.
<div style="border: 1px solid black; padding: 5px; text-align: center;"> MAINTEN. MODE </div>	<ul style="list-style-type: none"> ➤ Select "Maintenance MODE" by touching "↑" or "↓" switch. ➤ Touching "FUNC" switch when "MAINTEN. MODE" is displayed will enter Maintenance setting Mode. ➤ Measuring Condition will return on touching "RESET" switch.
<div style="border: 1px solid black; padding: 5px; text-align: center;"> CRO-SEN. [1.00]xG </div>	<ul style="list-style-type: none"> ➤ It sets the Cross sensitivity (0.1 ~ 5.0) of the sensor. ➤ Value setting is done by touching "↑" Switch or "↓" Switch by 0.01 units. ➤ Touching "FUNC" Switch will enter the next item.
<div style="border: 1px solid black; padding: 5px; text-align: center;"> Z-SKIP [0.0]%F </div>	<ul style="list-style-type: none"> ➤ It sets the Zero region sensitivity of the sensor. ➤ Value setting is done by touching "↑" Switch or "↓" Switch by 1 unit. ➤ The gas value less than corresponding setting is considered as 0; the setting is possible up to 10% of the High Scale. ➤ Touching "FUNC" Switch will enter the next item.
<div style="border: 1px solid black; padding: 5px; text-align: center;"> ODT [0]SEC </div>	<ul style="list-style-type: none"> ➤ It sets the Measuring Value delay depending on the set time.
<div style="border: 1px solid black; padding: 5px; text-align: center;"> AUTO-Z [ON] </div>	<ul style="list-style-type: none"> ➤ It sets whether to use Auto Zero function. ➤ Touching the "↑" or "↓" "Switch toggles" ON "and" OFF ". Auto zero function operates if it is ON (default is ON). ➤ If Auto Zero is ON, automatic Zero Calibration is performed when the value is maintained over 10 minutes less than 0.5% of variation within the values from Auto Zero minimum to 5% of the High Scale.
<div style="border: 1px solid black; padding: 5px; text-align: center;"> AZ MIN. [2.0]%F </div>	<ul style="list-style-type: none"> ➤ It sets the minimum value of Auto Zero. ➤ This Mode sets the percentage of High Scale in the range of 1.0%~4.0%. ➤ Touching "FUNC" Switch will enter the next item.
<div style="border: 1px solid black; padding: 5px; text-align: center;"> BASE-Z [ON] </div>	<ul style="list-style-type: none"> ➤ It sets whether to use Base Zero function. ➤ Touching the "↑" or "↓" "Switch toggles" ON "and" OFF ". Base zero function operates if it is ON (default is ON). ➤ If Base Zero is ON, automatic Zero Calibration is performed when the value is maintained over 10 minutes from 0.02% of the High Scale to Base Zero maximum. ➤ Touching "FUNC" Switch will enter the next item.

<div style="border: 2px solid black; padding: 5px; text-align: center;"> BZ MAX. [2.0]%F </div>	<ul style="list-style-type: none"> ➤ It sets the minimum value of Base Zero. ➤ This Mode sets the percentage of High Scale in the range of 0.5%~2.0%. ➤ Touching "FUNC" Switch will enter the next item.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> SP. HOLD [ON] </div>	<ul style="list-style-type: none"> ➤ It sets whether to use the function to HOLD the maximum value during SPAN Calibration. ➤ Touching the "↑" or "↓" Switch toggles ON "and" OFF ". Measuring Value HOLD function operates during Span Calibration if it is ON. ➤ Touching "FUNC" Switch will enter the next item.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> UNDER EN [OFF] </div>	<ul style="list-style-type: none"> ➤ It turns ON/OFF the Under Mode setting. ➤ Touching the "↑" or "↓" Switch toggles ON "and" OFF ". Under Mode is set when less than -10% of gas is measured if it is ON. ➤ If it is OFF, values under -10% will be processed as 0. ➤ Touching "FUNC" Switch will enter the next item.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> SEN CHK. [OFF] </div>	<ul style="list-style-type: none"> ➤ It sets whether to perform Combustible sensor check. ➤ Touching the "↑" or "↓" Switch toggles ON "and" OFF ". Whether the sensor is installed is automatically checked if it is ON. If it does not detect a sensor, Fault will be indicated. ➤ If it is OFF, sensor check is disabled. ➤ Touching "FUNC" Switch will enter the next item.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> S-DIR [INC] </div>	<ul style="list-style-type: none"> ➤ This item sets the direction of Sensor operation. ➤ Touching the "↑" Switch or "↓" Switch toggles the display of "INC" or "DEC". On INC, the Sensor operates to the direction of voltage/current increase; on DEC, to the direction of decrease. ➤ Touching "FUNC" Switch will enter the next item.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> S-DIR [DEC] </div>	
<div style="border: 2px solid black; padding: 5px; text-align: center;"> ENG MOD. [OFF] </div>	<ul style="list-style-type: none"> ➤ This item sets the display function of negative values of Gas Measuring Value. ➤ Touching the "↑" Switch or "↓" Switch toggles the ON/OFF status, If it is ON, negative value of Gas Measuring Value is displayed; OVER and UNDER Mode is not indicated; leftmost character in the 2nd row is expressed as '<'. MAINTENANCE MODE returns on touch of "FUNC" Switch.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> W / L TYPE [STEADY] </div>	<ul style="list-style-type: none"> ➤ This item is for setting the lighting method of the Warning Light in Normal condition. ➤ Green light is on with "STEADY"; green light will flash at 1 second interval with "BLINK."
<div style="border: 2px solid black; padding: 5px; text-align: center;"> M.- LEVEL [0] </div>	<ul style="list-style-type: none"> ➤ This item is for setting the current Output in Test Mode.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> EMC T/O [OFF] </div>	<ul style="list-style-type: none"> ➤ This item is for setting whether to set time in Test Mode. ➤ If it is ON, Test Mode is activated for 30 minutes only; if it is OFF, it is operated without restriction.

11.8. Device Mode setting

※  **Only authorized personnel are allowed to perform these settings.**

PASSWORD [**]	<ul style="list-style-type: none"> ➤ Touching "FUNC" switch with Magnet-bar for 2 seconds in Measuring Condition will enter the Password mode. ➤ Touch the "FUNC" switch after setting password using "↑" or "↓" switch.
DEVICE. MODE	<ul style="list-style-type: none"> ➤ Select "DEVICE MODE" by touching "↑" or "↓" switch. ➤ Touching "FUNC" switch when "DEVICE MODE" is displayed will enter DEVICE setting Mode. ➤ Measuring Condition will return on touching "RESET" switch.
HART B/D [CHECK]	<ul style="list-style-type: none"> ➤ This item is to check the connection status of HART BOARD. ➤ CHECK is displayed if connected; EMPTY if not.
PADD / mA 0 / EN.	<ul style="list-style-type: none"> ➤ This item is to check the Polling Address of HART device.
DEV-CODE [0xE1C3]	<ul style="list-style-type: none"> ➤ This item is to check the Unique ID of the HART device. ➤ Sensor ID cannot be changed since it is a unique ID of the product itself.
FIX CUR DISABLE	<ul style="list-style-type: none"> ➤ This item is to check the Fixed Current Mode of the HART device.
SERIA.NO *XXXXXXX	<ul style="list-style-type: none"> ➤ It is the Mode to check the Serial Number of the product.
TAG GTD-0001	<ul style="list-style-type: none"> ➤ This item is to check the Tag of the HART device. ➤ Modification is not possible in the Sensor.
LONG TAG [GTD-00>	<ul style="list-style-type: none"> ➤ This Mode is to check the Long Tag of the HART device. ➤ It is possible to check by shifting the string using "↑" Switch or "↓" Switch. ➤ Modification is not possible in the Sensor.
DESCRIP. [GASTRO>	<ul style="list-style-type: none"> ➤ This Mode is to check the Descriptor of the HART device. ➤ Modification is not possible in the Sensor.
MESSAGE [GASTRO>	<ul style="list-style-type: none"> ➤ This Mode is to check the Message of the HART device. ➤ Modification is not possible in the Sensor.

11.9. Version mode configuration

This Mode is to display the important revision information of the interior of the equipment.


<div style="border: 2px solid black; padding: 5px; text-align: center;"> PASSWORD [**] </div>	<ul style="list-style-type: none"> ➤ Touching "FUNC" switch with Magnet-bar for 2 seconds in Measuring Condition will enter the Password mode. ➤ Touch the "FUNC" switch after setting password using "↑" or "↓" switch.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> VERSION MODE </div>	<ul style="list-style-type: none"> ➤ Select "VERSION MODE" by touching "↑" or "↓" switch. ➤ Touching "FUNC" switch when "VERSION MODE" is displayed will enter VERSION setting Mode. ➤ Measuring Condition will return on touching "RESET" switch.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> FW REV [REV 6] </div>	<ul style="list-style-type: none"> ➤ It indicates the current version of the F/W.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> EX H/W [REV 2] </div>	<ul style="list-style-type: none"> ➤ It indicates the version of the H/W.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> HART DEV [REV 1] </div>	<ul style="list-style-type: none"> ➤ It indicates the version of the employed HART Device.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> HART REV [REV 7] </div>	<ul style="list-style-type: none"> ➤ It indicates the version of the employed HART Protocol. ➤ VERSION MODE will return on touching "FUNC" switch.

11.10. Test mode configuration

<div style="border: 2px solid black; padding: 5px; text-align: center;"> PASSWORD [**] </div>	<ul style="list-style-type: none"> ➤ Touching "FUNC" switch with Magnet-bar for 2 seconds in Measuring Condition will enter the Password mode. ➤ Touch the "FUNC" switch after setting password using "↑" or "↓" switch.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> TEST MODE </div>	<ul style="list-style-type: none"> ➤ Select "TEST MODE" by touching "↑" or "↓" switch. ➤ Touching "FUNC" switch when "TEST MODE" is displayed will enter TEST setting Mode. ➤ Measuring Condition will return on touching "RESET" switch.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> mA OUT [OFF] </div>	<ul style="list-style-type: none"> ➤ This item sets whether to include mA Output during the TEST. ➤ Touching the "↑" or "↓" Switch will toggle the ON/OFF status; if it is ON, mA will be output by the setting value during TEST.
<div style="border: 2px solid black; padding: 5px; text-align: center;"> [TEST] [0] </div>	<ul style="list-style-type: none"> ➤ This item performs the TEST. ➤ Test Gas value is set by touching "↑" or "↓" Switch; if the mA Output is ON, the mA Output is displayed coupled with Test Gas value. ➤ TEST MODE will return on touching "FUNC" switch.

11.11. Inspection mode use

This Mode is used for the inspector to identify the Sensor status and Fault details without affecting the equipment operated in emergency. Only authorized personnel are allowed to use this Mode.



- Press and hold the "↓" Switch for at least 3 seconds while Means value display gas concentrations in the display. Press and hold the "↓" Switch for at least 3 seconds to exit again.
- Entering Inspection Mode, '#' mark will flash at the first place in the second row.
- You can enter M/L item from Maintenance Mode to set Output value.

11.12. Data initialization


Only authorized personnel are allowed to conduct this Mode because it will initialize all the values to the data set in the factory before shipping.



- Turn the power ON while holding "FUNC" Key and "UP" Key.
- When "ALL - INIT" is displayed on the Display window, select "YES" to carry out the data initialization.

11.13. Correction data initialization

Only authorized personnel is allowed to conduct the initialization because this Mode initializes to the value of Calibration data set in the factory before shipping. This Mode is used for the inspector to initialize only the Calibration value among setting values.



- Turn the power ON while holding "FUNC" Key and "UP" Key.
- When "CAL - INIT" is displayed on the Display window, select "YES" to carry out the normal initialization of Calibration data.

12. Troubleshooting

Fault code / Output Message	Description & Condition	Recovery
FAULT1 "SEN EMPT"	Occurs when Combustible sensor module is not connected.	sensor module connect fault
FAULT2 "SEN HIGH"	When Combustible sensor Output is over the maximum ADC value.	sensor module fault or transmitter Board ADC fault
FAULT3 "SEN LOW"	When Combustible sensor Output is under the minimum ADC value.	sensor module fault or transmitter Board ADC fault
FAULT4 "EROM ERR"	transmitter EEPROM Checksum fault	transmitter Board EEPROM fault
FAULT5 "+24V LOW"	Occurs when 24V main power input is less than 10V.	Power supply input voltage confirm & transmitter ADC fault
FAULT6 "ADC FAIL"	transmitter ADC fault	transmitter ADC fault
FAULT7 "H/W REV"	H/W version error	Check transmitter ADC resistance

13. Caution before installation

13.1. Selection of installation location (Occupational Safety and Health Law)

The Gas leak detection alarm system shall be installed in such place as follows. :

- 1) Near chemical accessory equipment installed inside/outside of a building and susceptible of gas leak such as compressors, valves, reactors, and piping connections, etc. dealing with combustible and toxic materials.
- 2) Locations risky of remaining gas near manufacturing equipments with ignition source like heaters.
- 3) Around connections of filling equipments of combustible and toxic substances.
- 4) Substations, distribution panel rooms, control rooms, etc. near explosion-proof area.
- 5) Other special gas-friendly places.

13.2. Selection of installation location (High Pressure Gas Safety Management Regulations)


The Gas detector of the Gas leak detection alarm system shall be installed close to risky area of gas leakage. However, if the direct gas leaks are not expected, but gas residence is vulnerable, it should be installed in such places as follows.

- 1) A gas leak detection alarm outside of a building shall be installed in a risky place of gas residence considering the wind direction, wind speed, and the gravity of the gas.
- 2) A gas leak detection alarm inside of a building shall be installed in the lower part of the building if the gas is lighter than the air, and upper part or near the vent of the building.
- 3) The alarm of the Gas leak detection alarm system shall be installed near Gas detector or in places where workers usually are.


13.3. Precaution before installation

Rainwater shall be avoided because it can be an electrical hindrance, and accessibility should be considered for periodic maintenance before installation. Vibration or shock shall be avoided since it may affect the output value, and the sensor shall face the direction of gravity when installed.

- This device has high pressure explosion-proof structure; belongs to GROUP II targeting gas and steam from general workplaces and chemical plants; and can be used in hazardous places of ZONE 1 (ONE) –class 1 and ZONE 2 (TWO) –class 2.
- Allowable temperature belongs to 85 °C or lower, which corresponds to T6.
- The ambient temperature shall be in the range of -20 °C ~ 60 °C.
- Installation elevation: less than 1,000 M above sea level
- Relative Humidity: 5-99%
- Installation place: indoors or outdoors
- Explosive ignition temperature of the gases or vapors used: Ex d IIC T6
- The wire conduit shall be sealed to prevent the gas moving or the explosion flame propagation through the conduit under 45cm when the explosion-proof cable gland is used at the cable inlet or when metal conduit is used in wiring works.
- At least 5 screw threads must be used for connection of this device and the conduit.
- Other standards should be met in this work such as: [Standards on the selection, installation and maintenance of wiring for workplace explosion-proof structural electrical mechanism].
- **Only qualified materials shall be used in cable entry including CABLE GLAND and SEALING FITTING; and used in the closure of unused incoming part.**

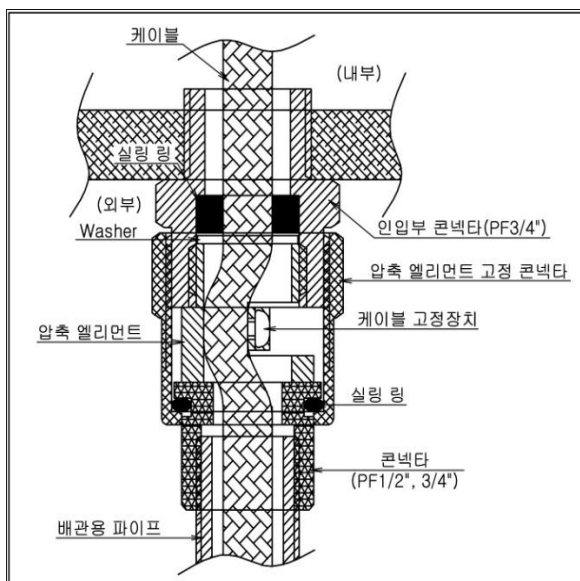

[Figure 13. Pressure packing type]

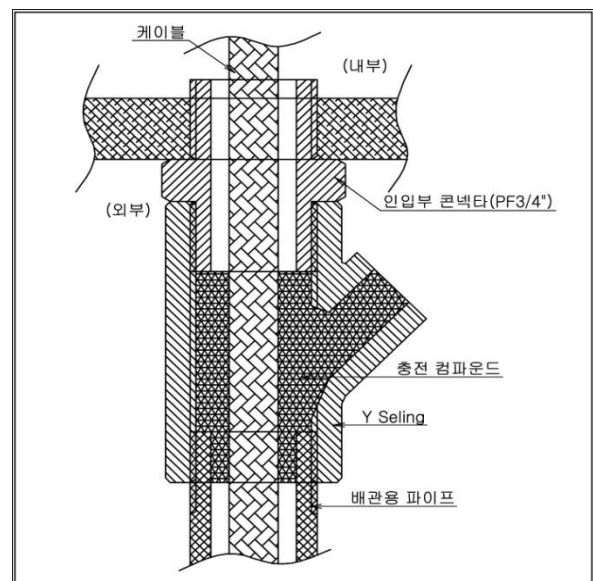

[Figure 14. Y Sealing Compound]

14. Ordering Information

GAS NAME		MESURING RANGE	TLV-TWA
Acetic Acid	CH_3COOH	0 ~ 30 ppm	10 ppm
Ammonia	NH_3	0 ~ 75 ppm	25 ppm
Antimony Pentachloride	SbCl_5	0 ~ 15 ppm	5 ppm
Arsetic Tafluoride	AsF_3	0 ~ 9 ppm	3 ppm
Arsetic Pentafluoride	AsF_5	0 ~ 9 ppm	3 ppm
Arsenic Trichloride	AsCl_3	0 ~ 15 ppm	5 ppm
Arsenic Pentachloride	AsCl_5	0 ~ 15 ppm	5 ppm
Arsine	AsH_3	0 ~ 0.3 ppm	0.05 ppm
Boron Trichloride	BCl_3	0 ~ 15 ppm	5 ppm
Boron Tribromide	BBr_3	0 ~ 9 ppm	3 ppm
Boron Trifluoride	BF_3	0 ~ 9 ppm	3 ppm
Bromine	Br_2	0 ~ 1 ppm	0.1 ppm
Chlorine	Cl_2	0 ~ 3 ppm	1 ppm
Carbon Tetrachloride	CCl_4	0 ~ 30 ppm	5 ppm
Carbon Monoxide	CO	0 ~ 150 ppm	25 ppm
Chlorine Tetrafluoride	ClF_3	0 ~ 1 ppm	0.1 ppm
Diborane	B_2F_6	0 ~ 0.3 ppm	0.1 ppm
Dichlorosilane	SiH_2Cl_2	0 ~ 15 ppm	5 ppm
Disilane	Si_2H_6	0 ~ 15 ppm	5 ppm
Ethylene Oxide	$\text{C}_2\text{H}_4\text{O}$	0~30ppm	1ppm
Fluorine	F_2	0 ~ 3 ppm	1 ppm
Germane	GeH_4	0 ~ 2 ppm	0.2 ppm
Germanium Tetrachloride	GeCl_4	0 ~ 15 ppm	5 ppm
Hydrazine	N_2H_4	0 ~ 10 ppm	0.01 ppm
Hydrogen	H_2	0 ~ 2000 ppm	LEL=4%VOL
Hydrogen Bromide	HBr	0 ~ 9 ppm	3 ppm
Hydrogen Chloride	HCl	0 ~ 15 ppm	5 ppm
Hydrogen Cyanide	HCN	0 ~ 30 ppm	10 ppm
Hydrogen Fluoride	HF	0 ~ 9 ppm	3 ppm
Hydrogen Iodine	HI	0 ~ 5 ppm	2 ppm
Hydrogen Selenide	H_2Se	0 ~ 0.2 ppm	0.05 ppm
Hydrogen Sulfide	H_2S	0 ~ 30 ppm	10 ppm
Iodine	I_2	0 ~ 1 ppm	0.1 ppm
Isopropyl Alcohol(IPA)	$\text{CH}_3\text{CHOHCH}_3$	0 ~ 2000 ppm	400 ppm
Molybdenum Fluoride	MoF_6	0 ~ 9 ppm	3 ppm
Nitric Acid	HNO_3	0 ~ 20 ppm	2 ppm
Nitrogen Monoxide	NO	0 ~ 100 ppm	25 ppm
Nitrogen Dioxide	NO_2	0 ~ 15 ppm	3 ppm
Nitrogen Trifluoride	NF_3	0 ~ 30 ppm	10 ppm
Nitrogen Tetraoxide	N_2O_4	0 ~ 15 ppm	3 ppm
Oxygen	O_2	0 ~ 25% Volume	-
Ozone	O_3	0 ~ 1 ppm	0.1 ppm

GAS NAME		MESURING RANGE	TLV-TWA
Phosgene	COCl_2	0 ~ 0.3 ppm	0.1 ppm
Phosphine	PH_3	0 ~ 1 ppm	0.3 ppm
Phosphorus Oxychloride	POCl_3	0 ~ 15 ppm	5 ppm
Phosphorus Pentafluoride	PF_5	0 ~ 9 ppm	3 ppm
Phosphorus Trichloride	PCl_3	0 ~ 15 ppm	5 ppm
Silane	SiH_4	0 ~ 15 ppm	5 ppm
Silicon Tetrachloride	SiCl_4	0 ~ 15 ppm	5 ppm
Silicon Tetrafluoride	SiF_4	0 ~ 9 ppm	3 ppm
Sulfur Dioxide	SO_2	0 ~ 10 ppm	2 ppm
Sulfur Tetrafluoride	SF_4	0 ~ 9 ppm	3 ppm
Sulfur Hexafluoride	SF_6	0 ~ 2000 ppm	
Tantalum Fluoride	TaF_5	0 ~ 9 ppm	3 ppm
Tetraethyl Orthosilicate	TEOS	0 ~ 15 ppm	10 ppm
Tin Tetrachloride	SnCl_4	0 ~ 15 ppm	5 ppm
Titanium Fluoride	TiF_4	0 ~ 9 ppm	3 ppm
Titanium Tetrachloride	TiCl_4	0 ~ 15 ppm	5 ppm
Trichlorosilane	SiHCl_3	0 ~ 15 ppm	5 ppm
Trimethoxy Phosphate	$\text{P}(\text{OCH}_3)_3$	0 ~ 15 ppm	2 ppm
Tungsten Hexafluoride	WF_6	0 ~ 9 ppm	3 ppm

15. Revision history

Version	Contents	Date
0	* Initial revision of the Manual	JUL. 31 , 2012
1	* Spec. revised(Added power consumption), Revised company address.	JAN 23, 2013
END		

This product and instruction manual are subject to change without prior notice for the improvement of product performance and ease of use.



Gastron Co., Ltd.

**Address: 18-8 Dogeumdanji 1gil(Palgogi-dong), Sanglok-gu,
Ansan-city, Gyeonggi-do, Korea,**

Tel : 031-490-0800

Fax : 031-490-0801

<http://www.gastron.com>

business@gastron.com